HITACHI S-9220

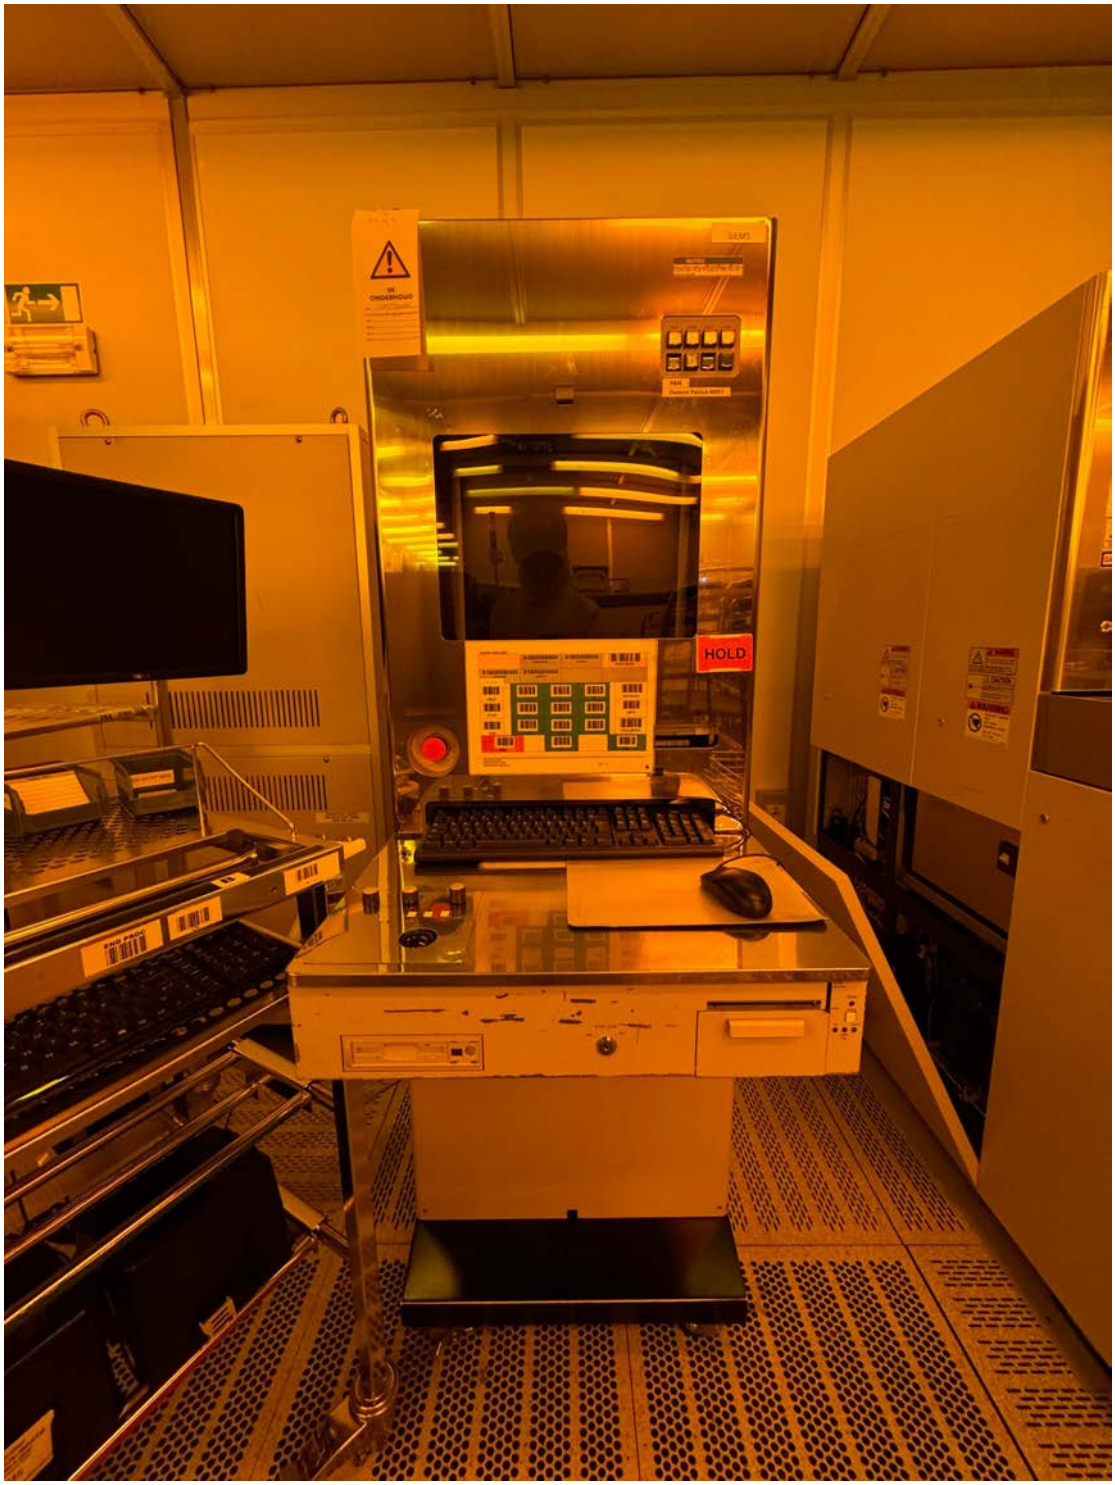
HOLD

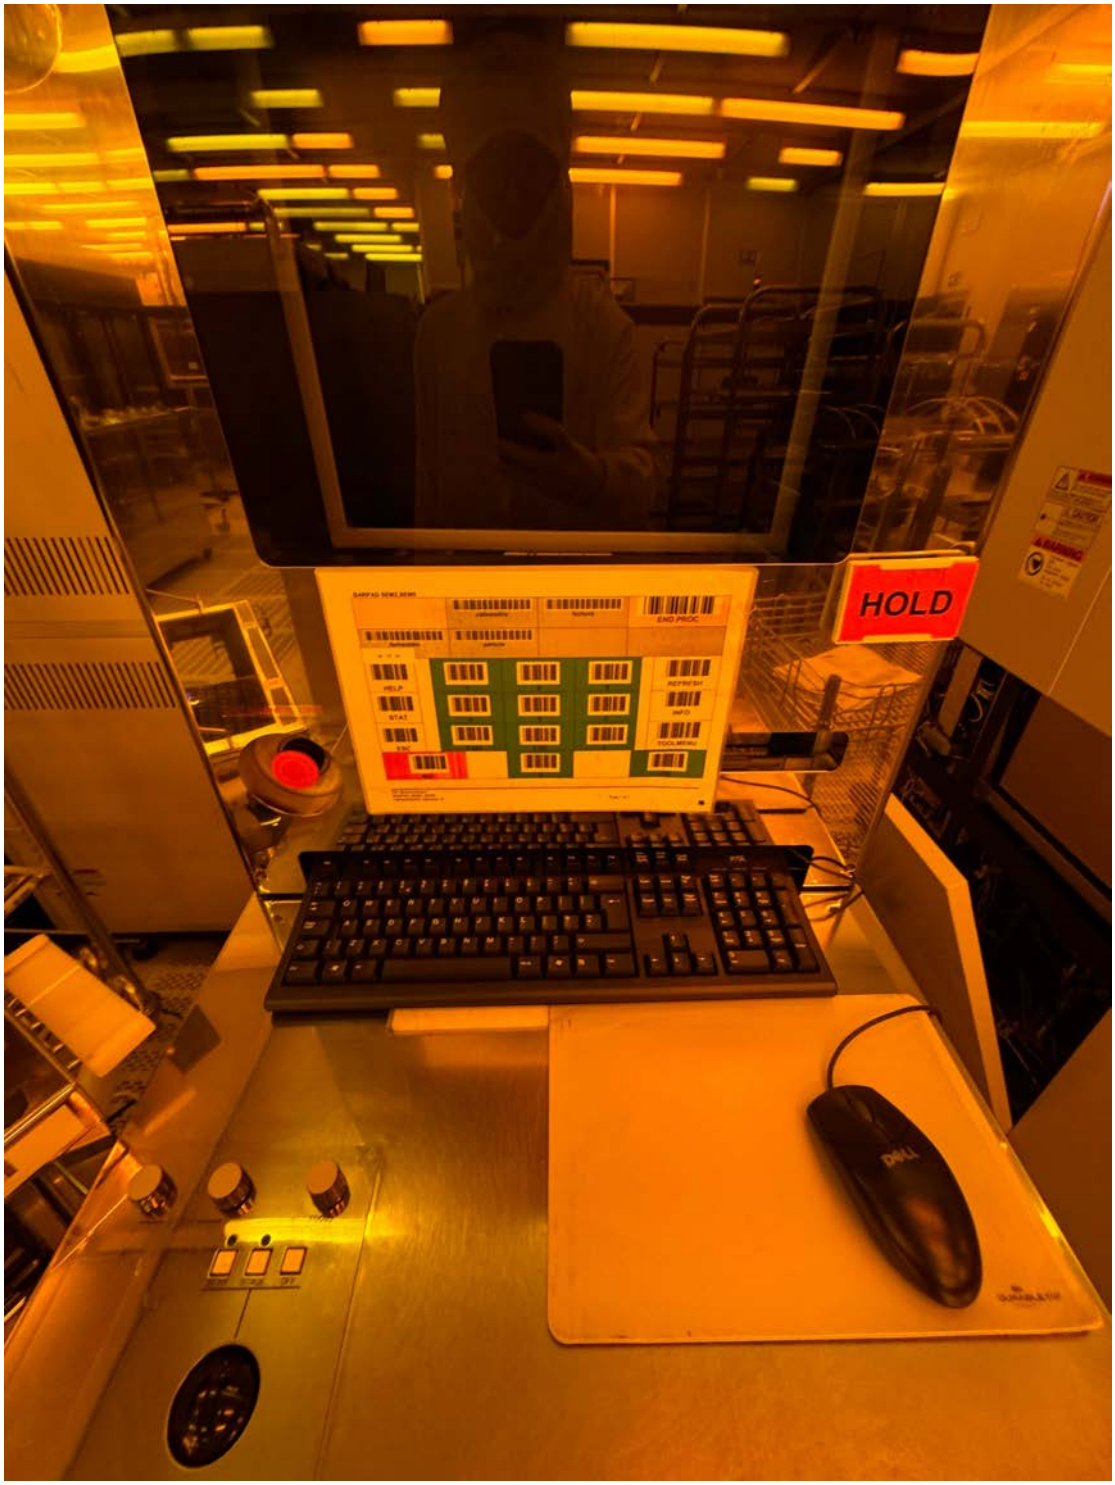
HOLD

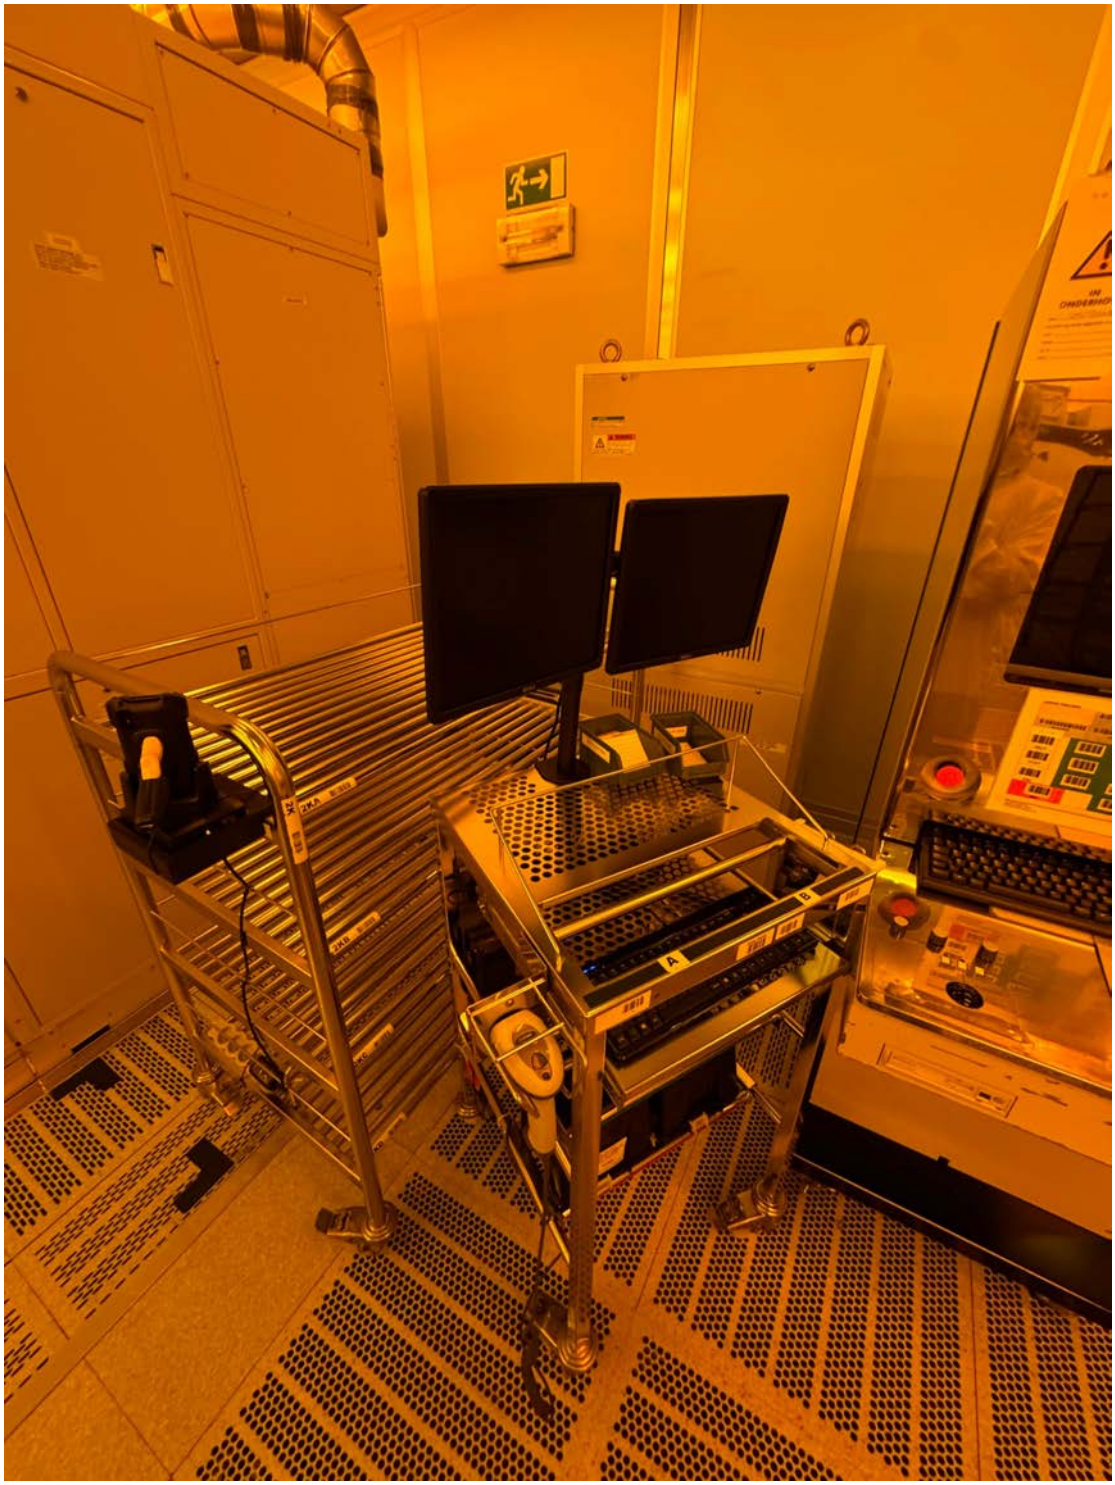

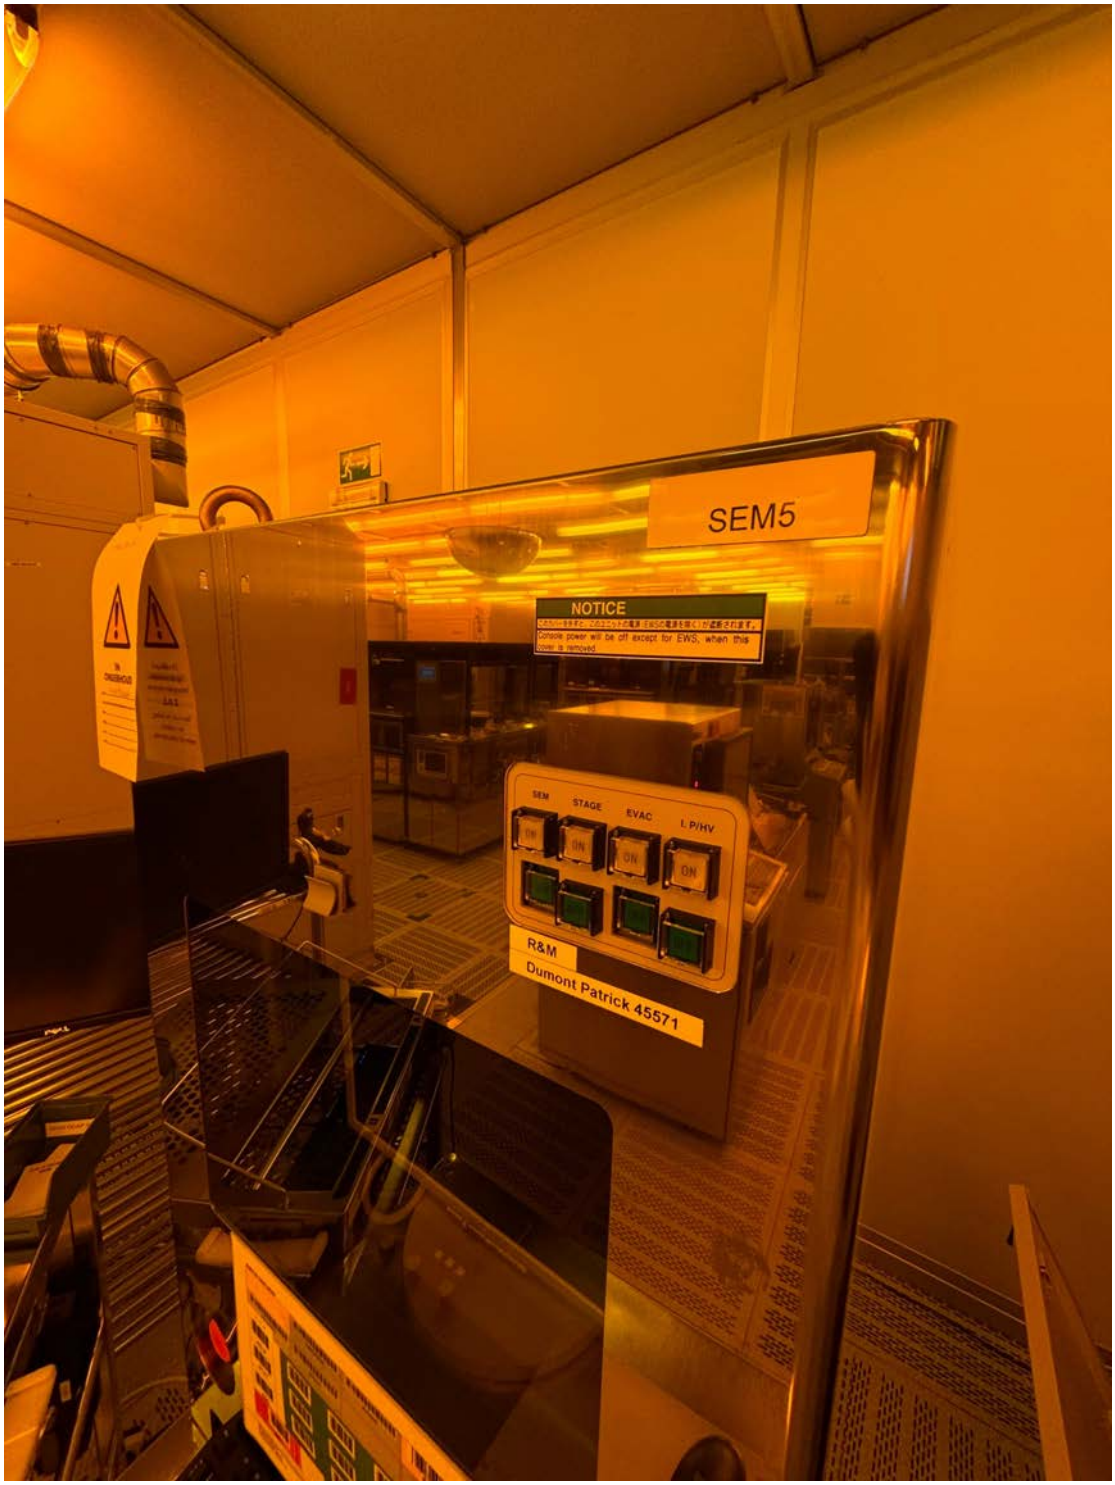
SEM5
NOTICE
SEM
STAGE
EVAC
I. P/HV
ON
R&M
Dumont Patrick 45571

Con. login: cdsem, hid
Login: mainte, propro

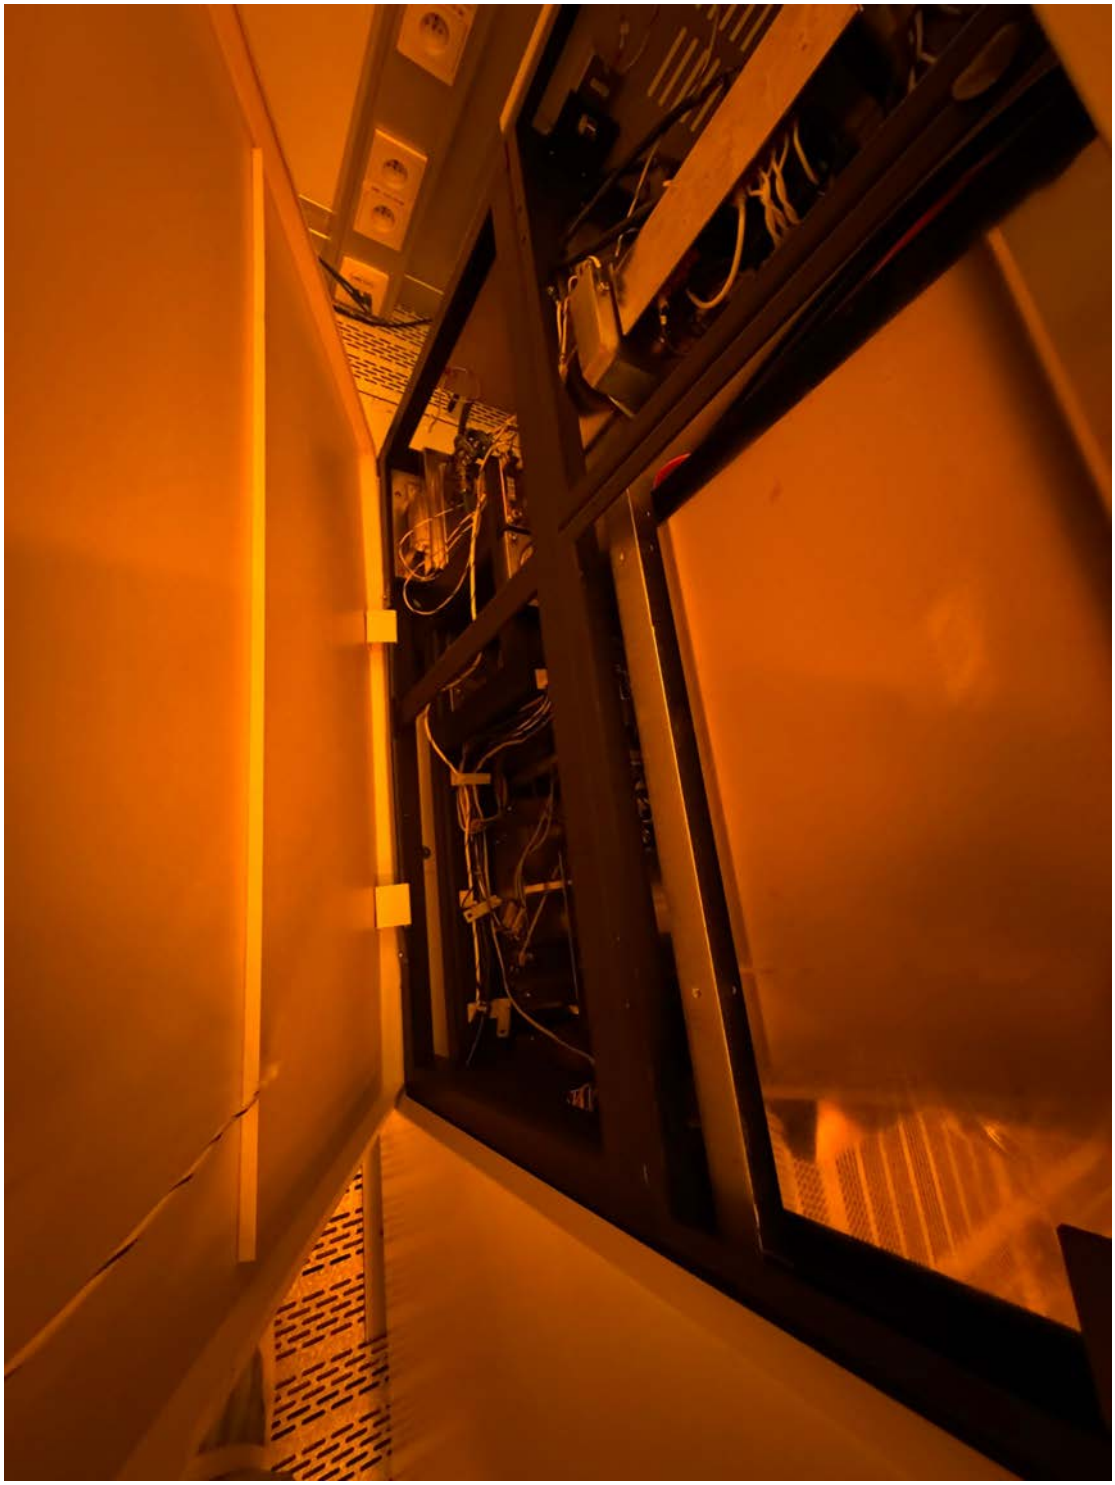

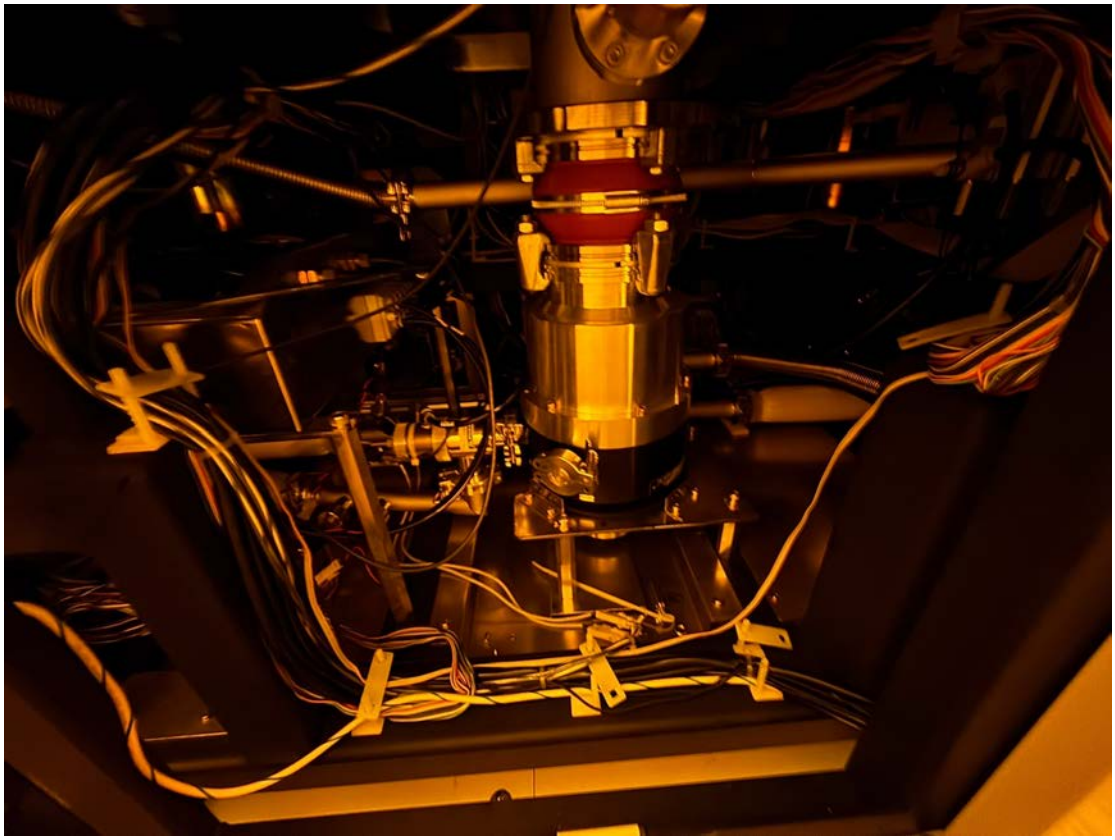

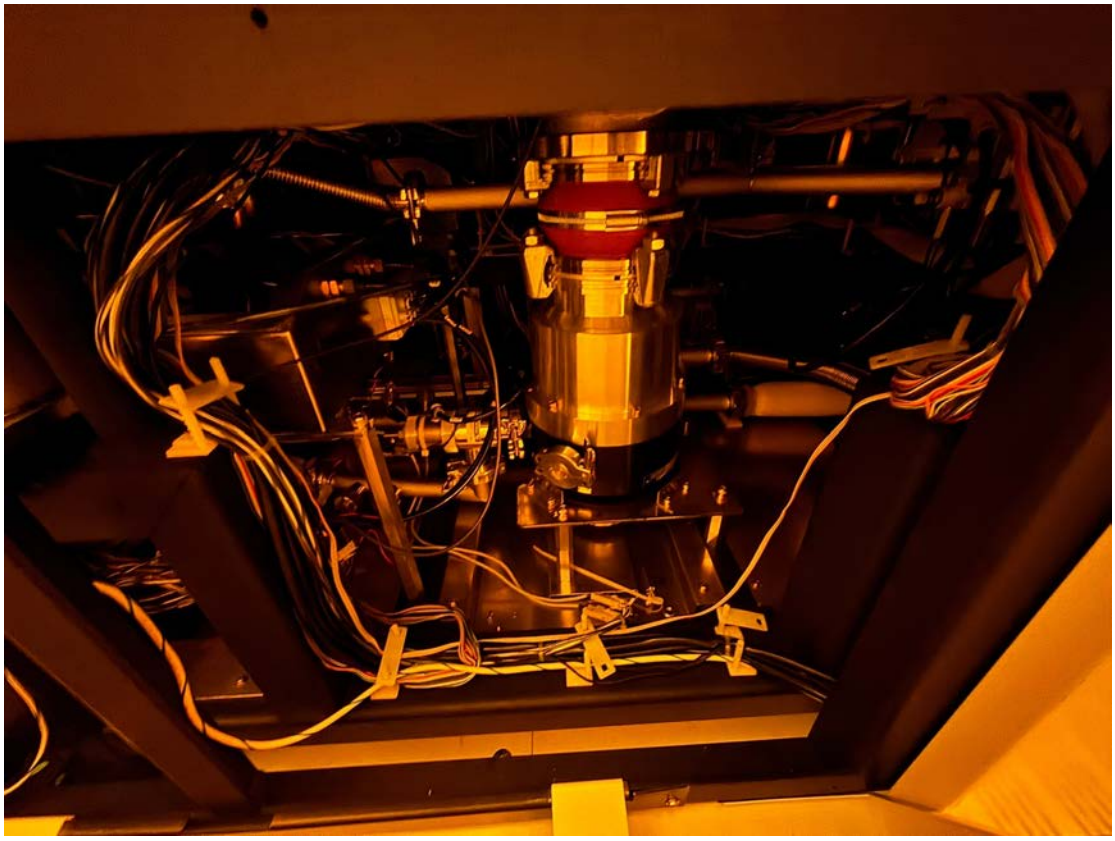

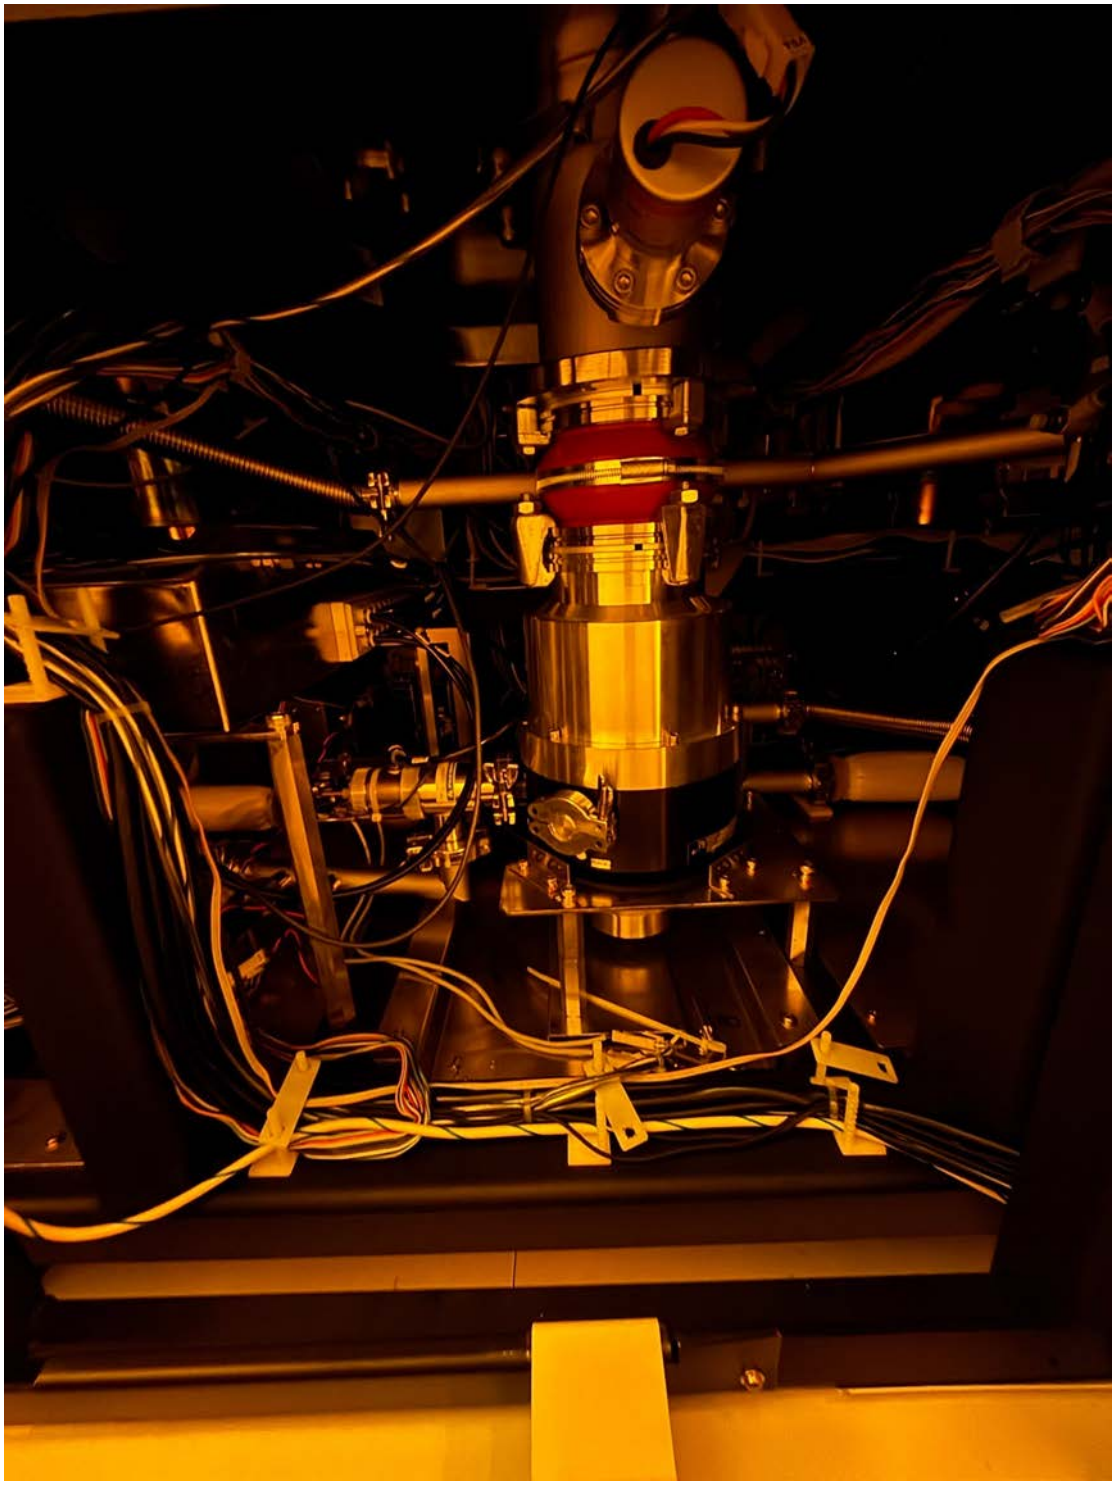

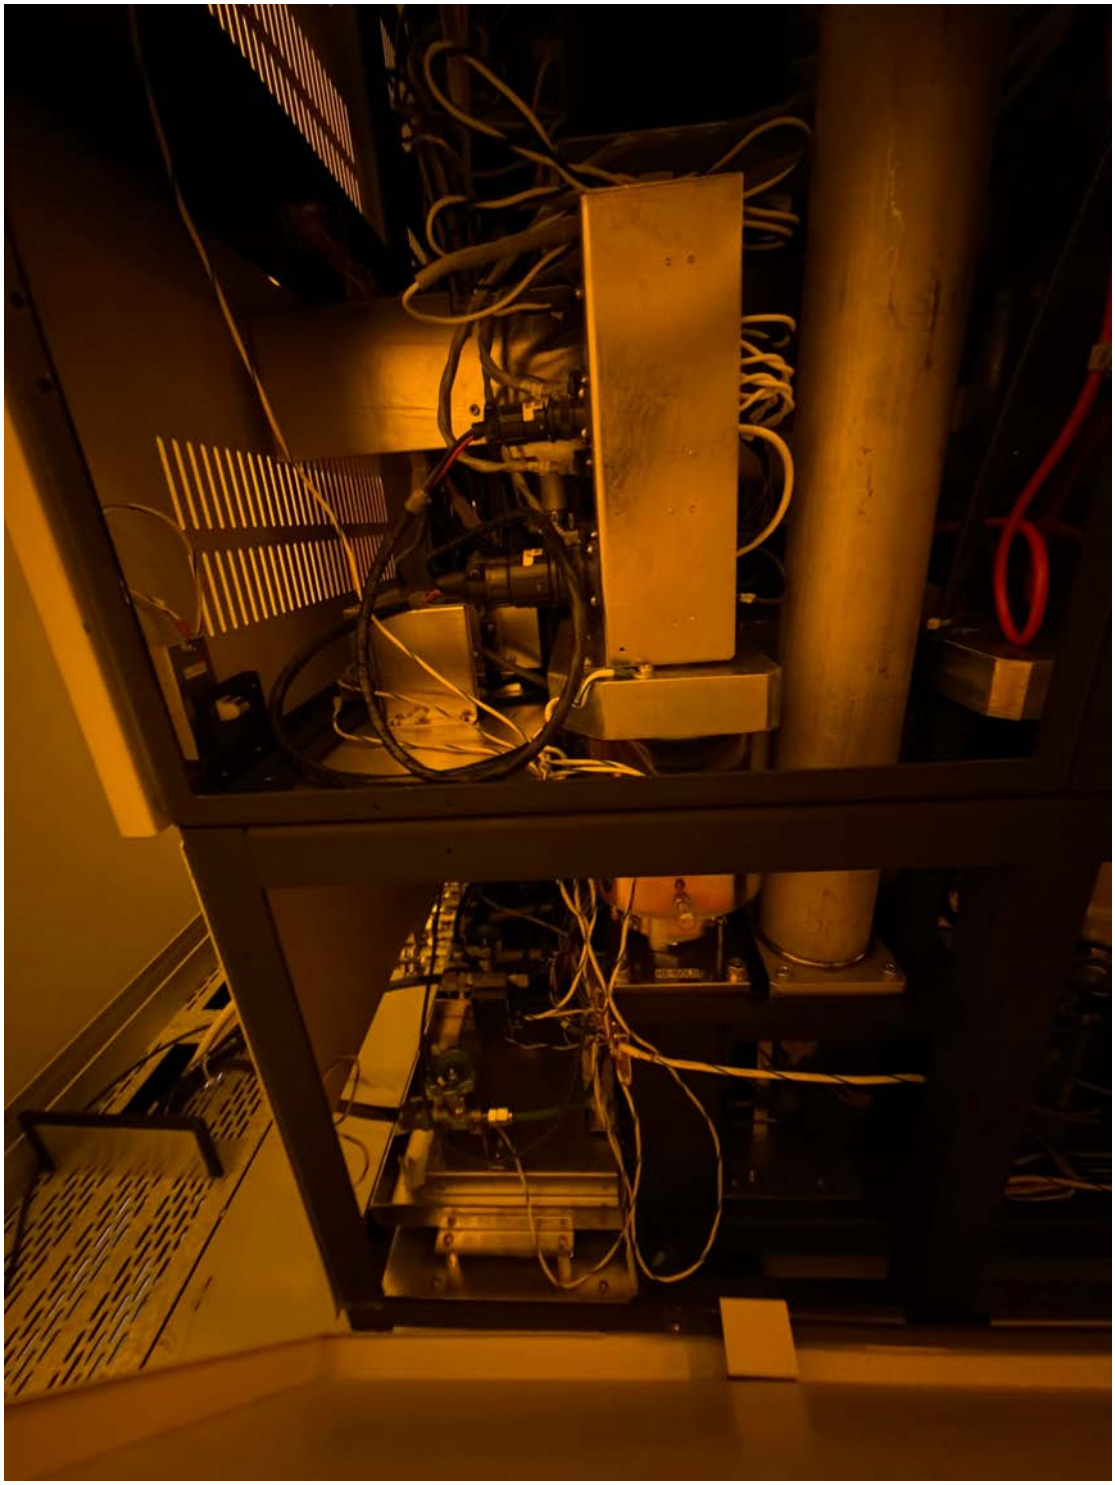

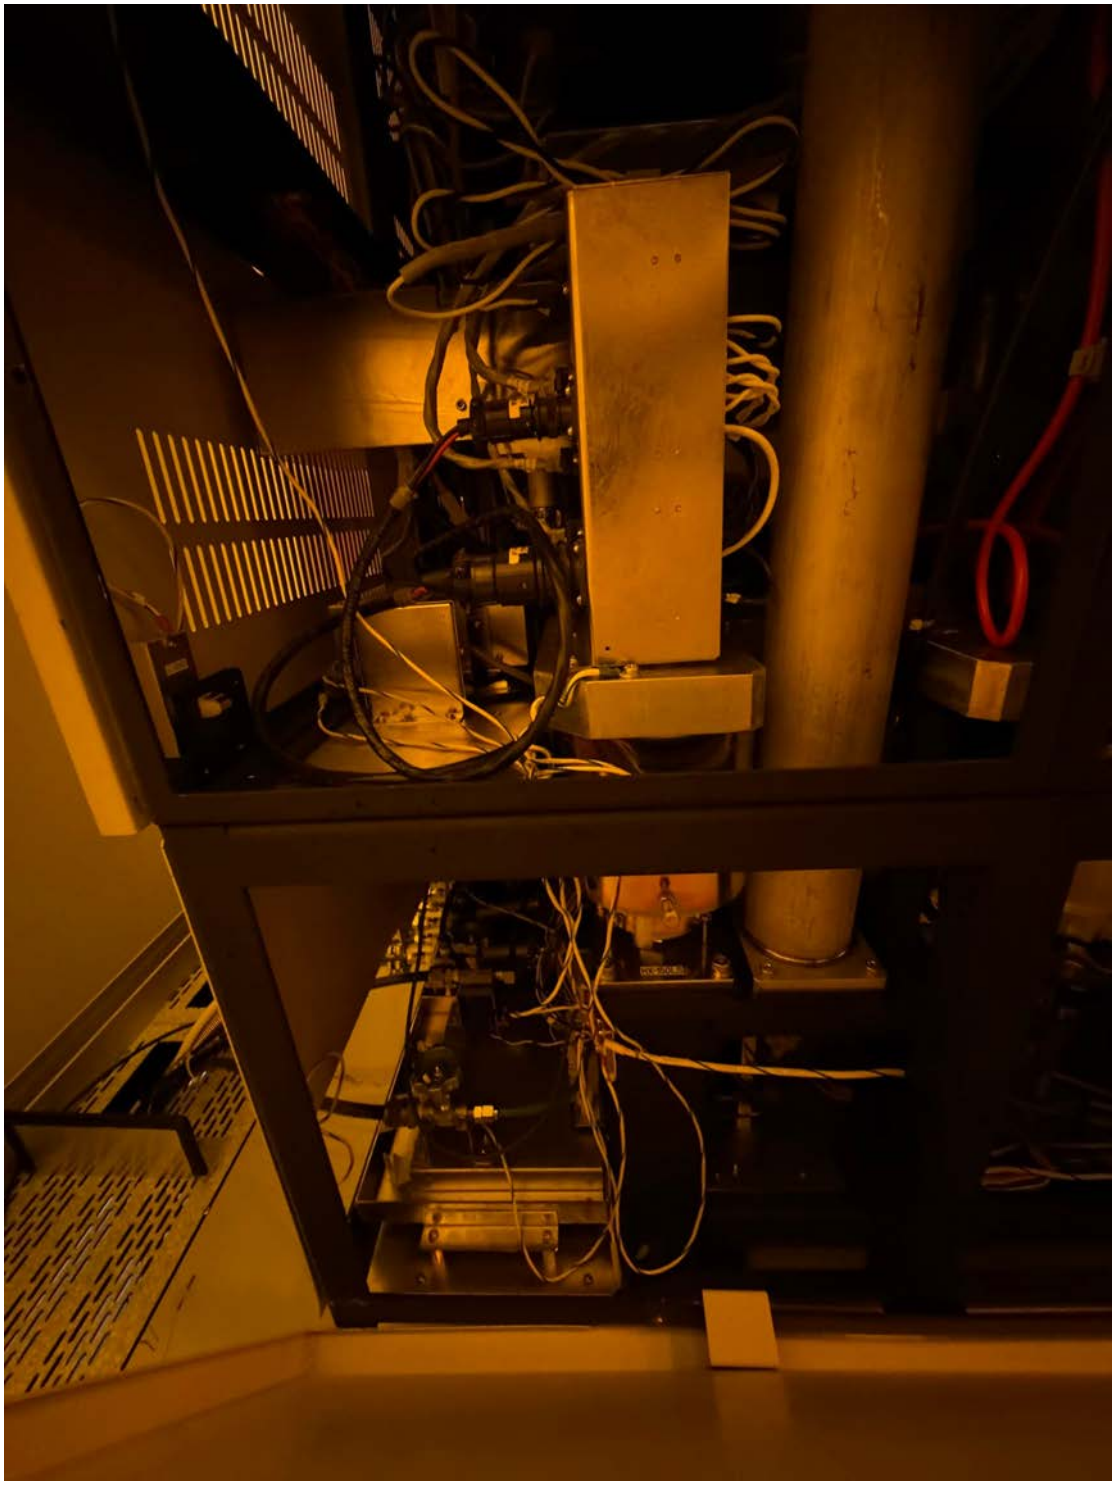

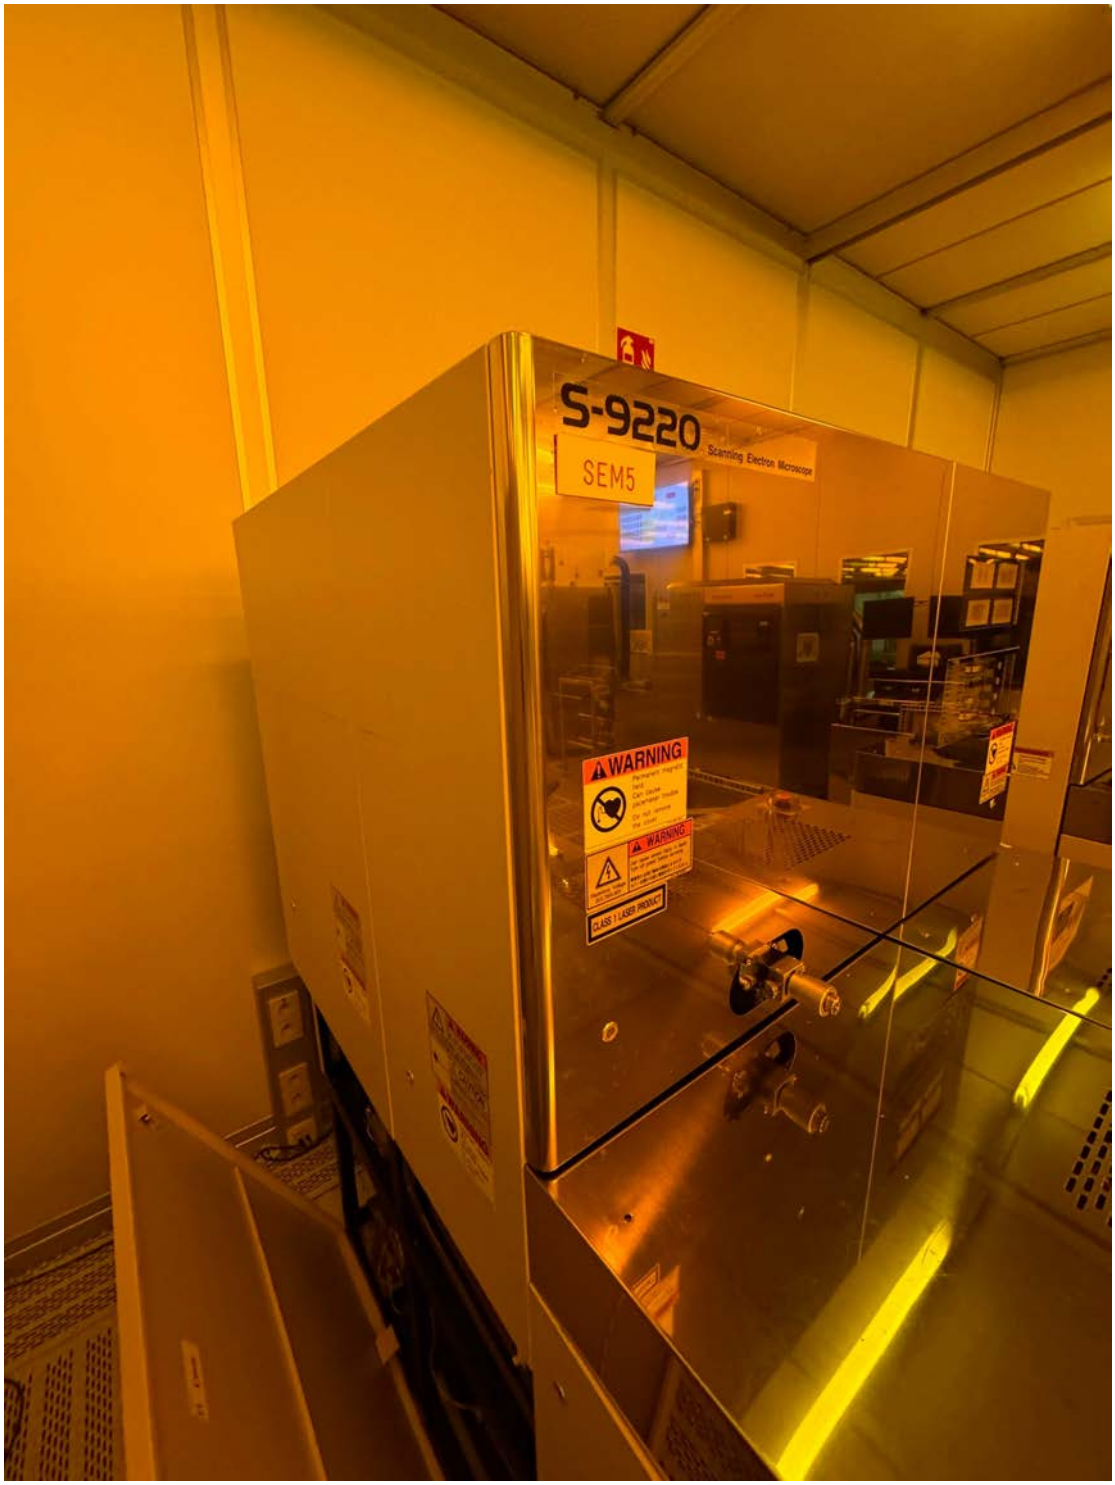
S-9220
Scanning Electron Microscope
SEM5
WARNING
WARNING
CLASS 1 LASER PRODUCT

S-9220
HITACHI

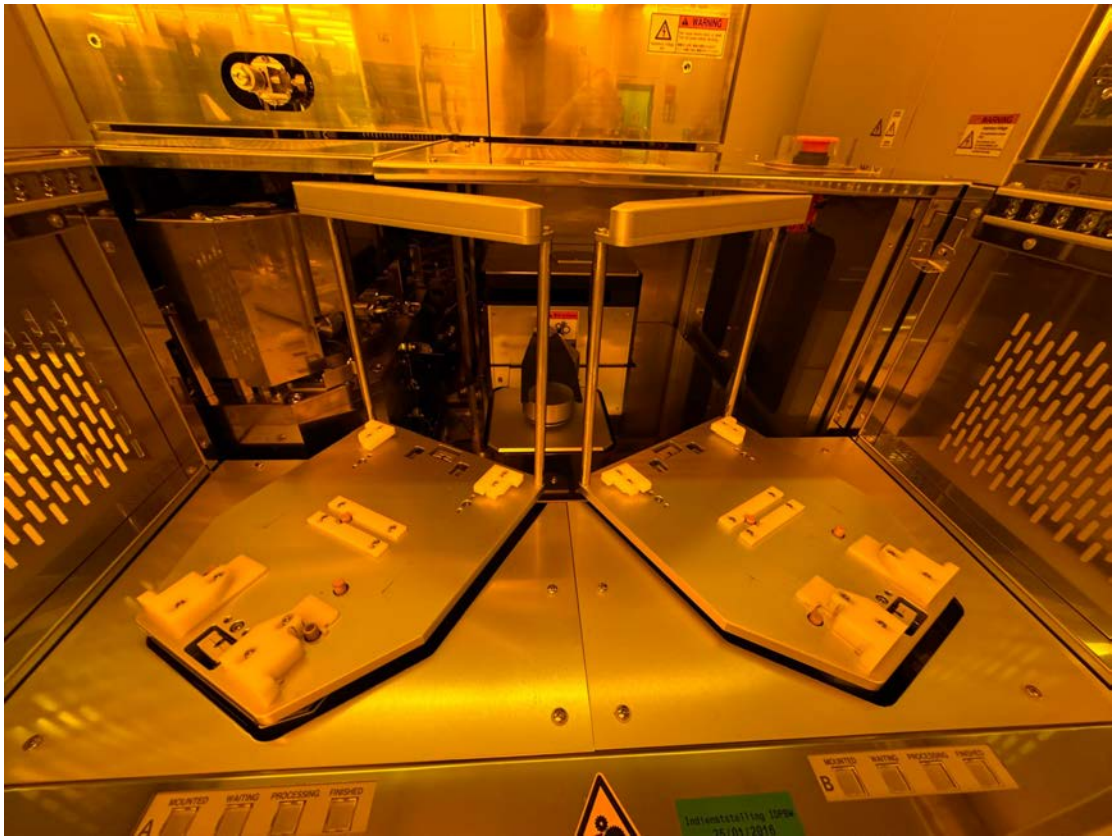
WARNING
MOUNTED
WAITING
PROCESSING
FINISHED

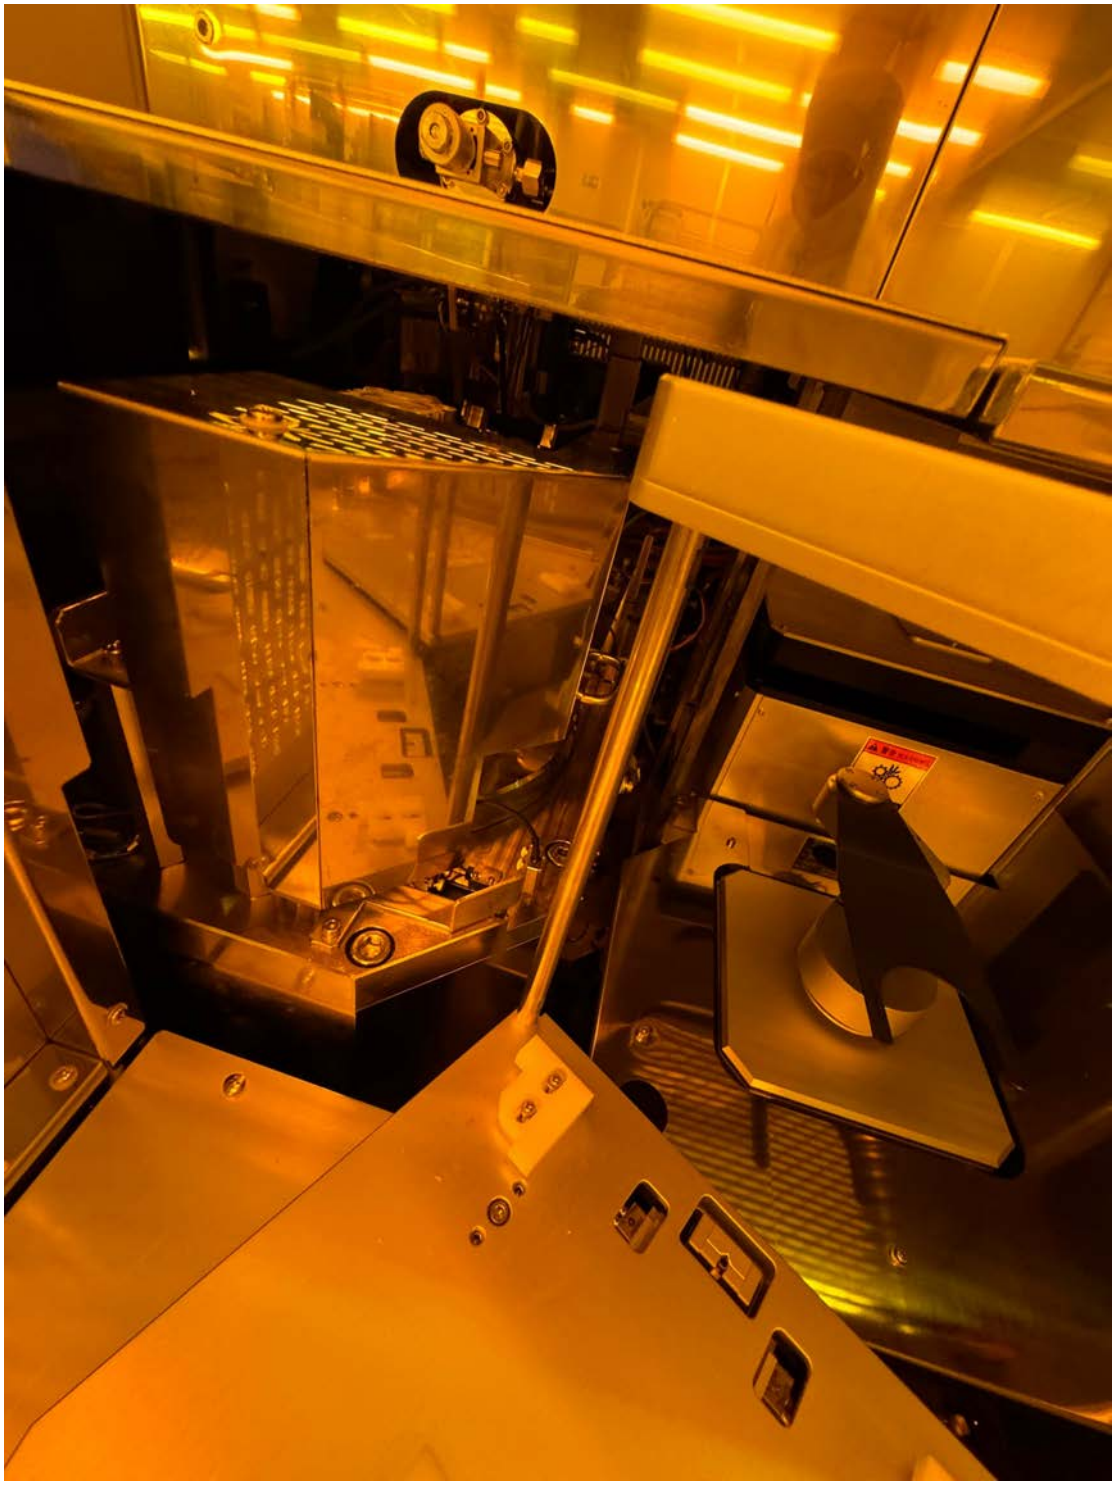

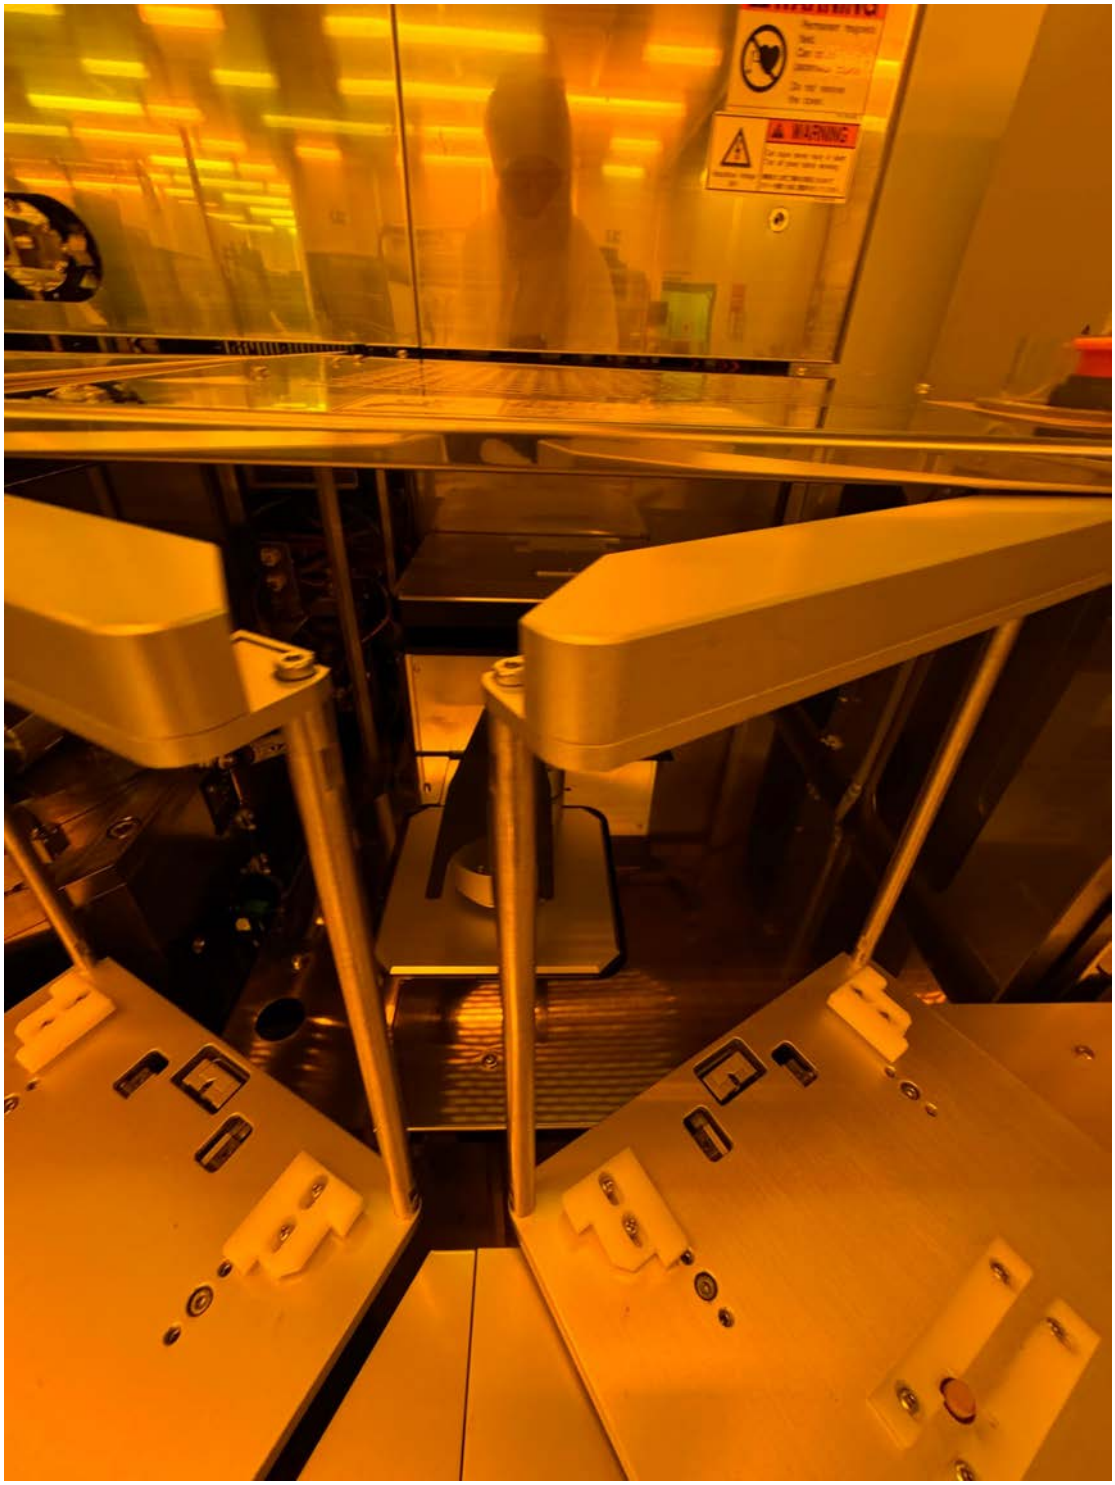
WARNING

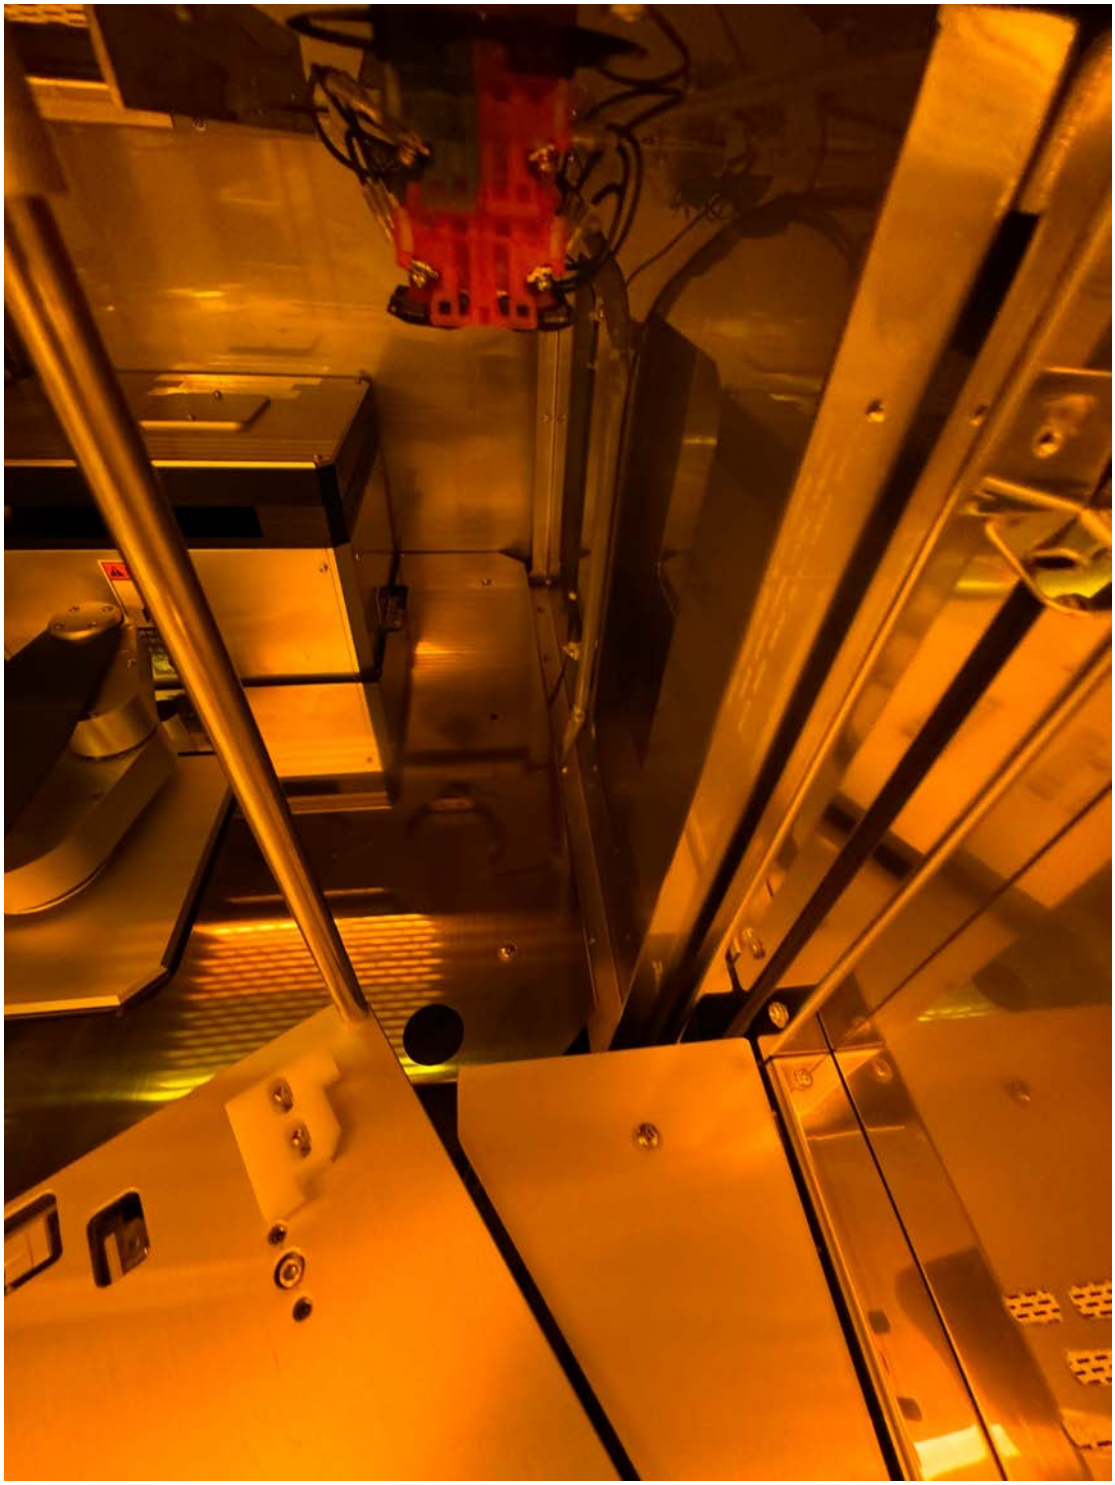

H V
BAKING
WARNING
WARNING

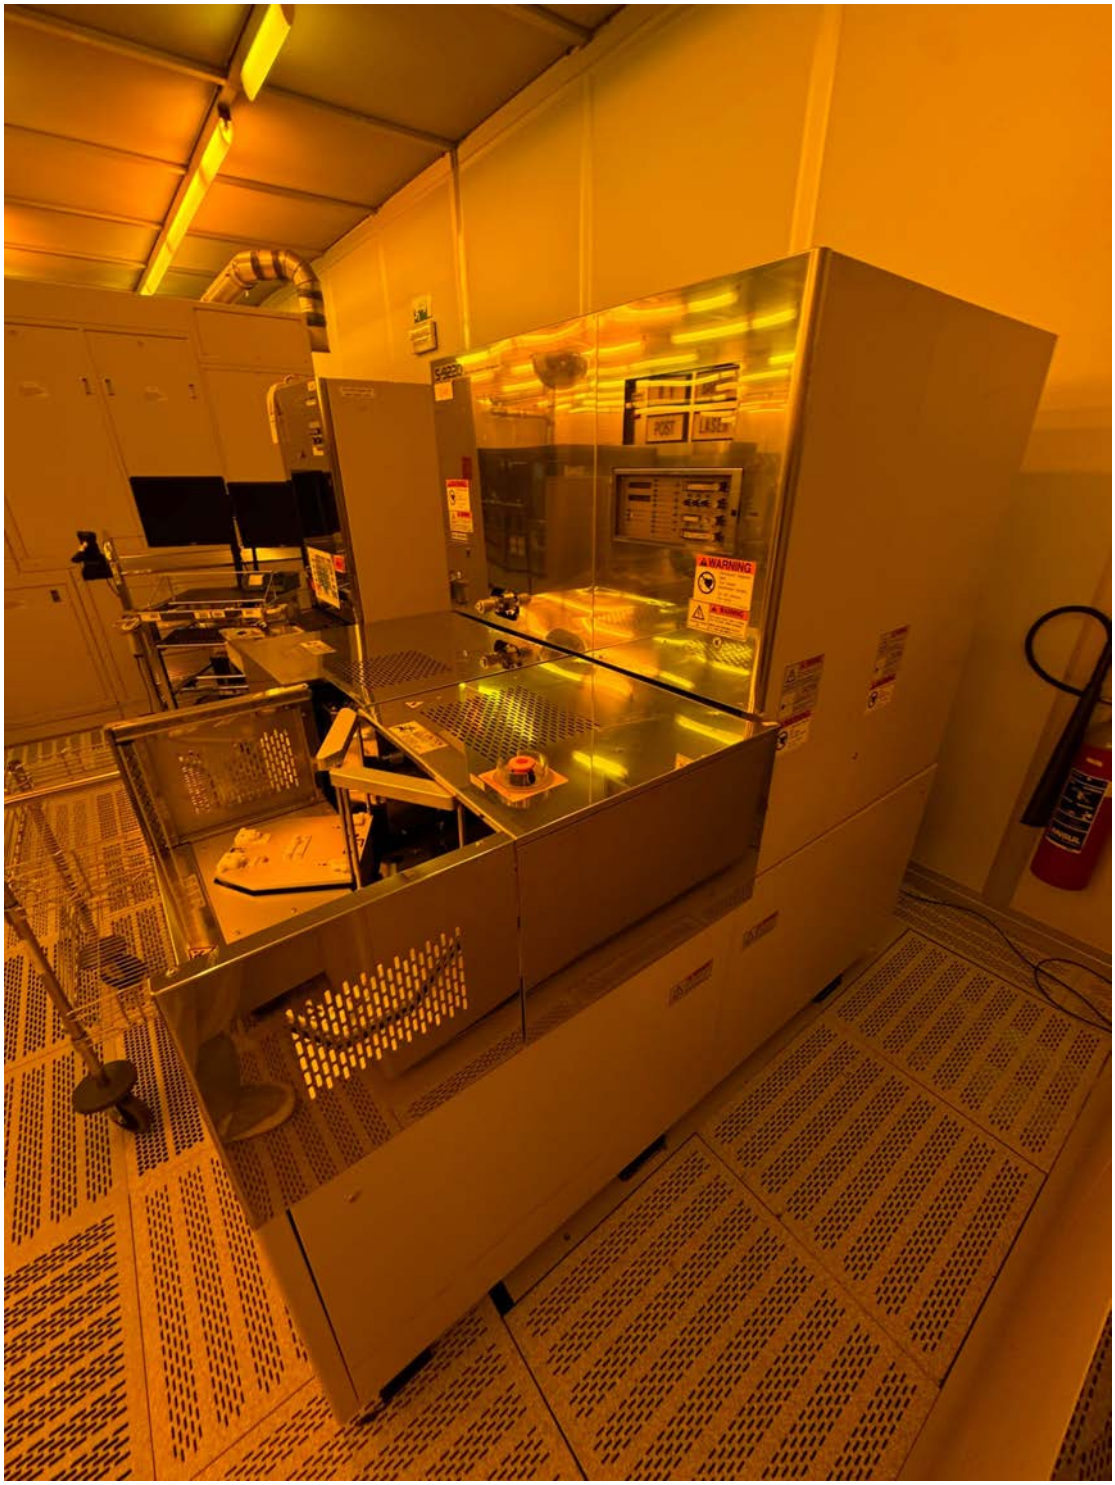
WARNING

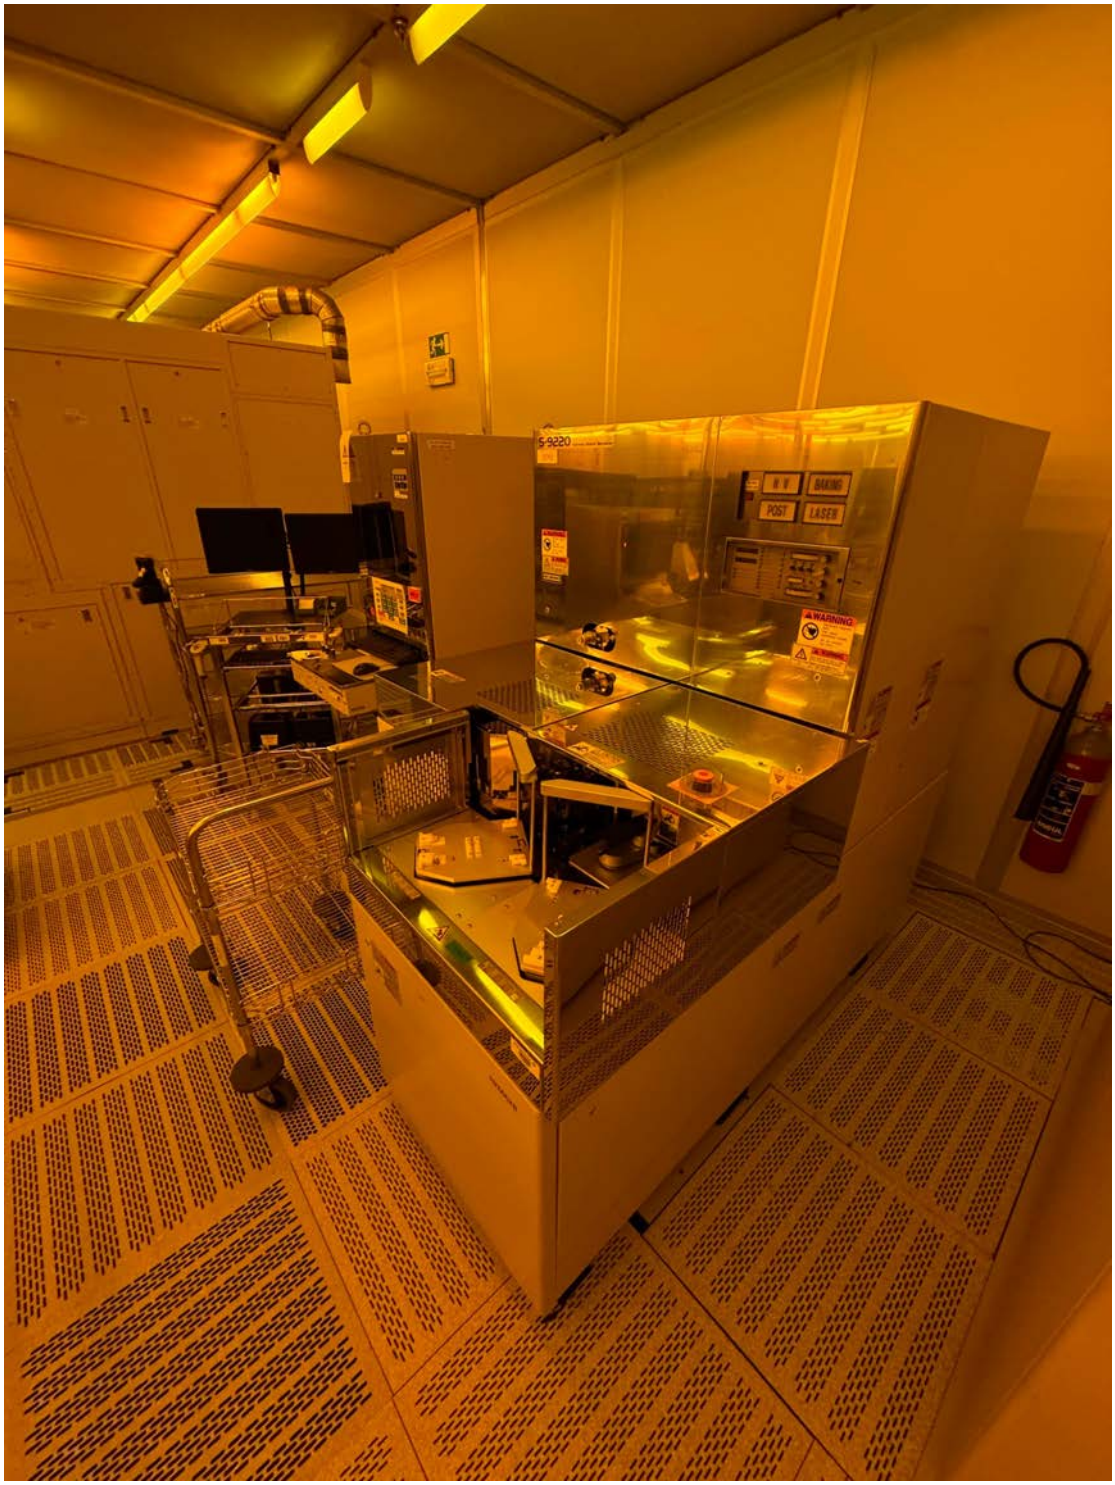
S-9220
N V
BAKING
POST
LASER
WARNING

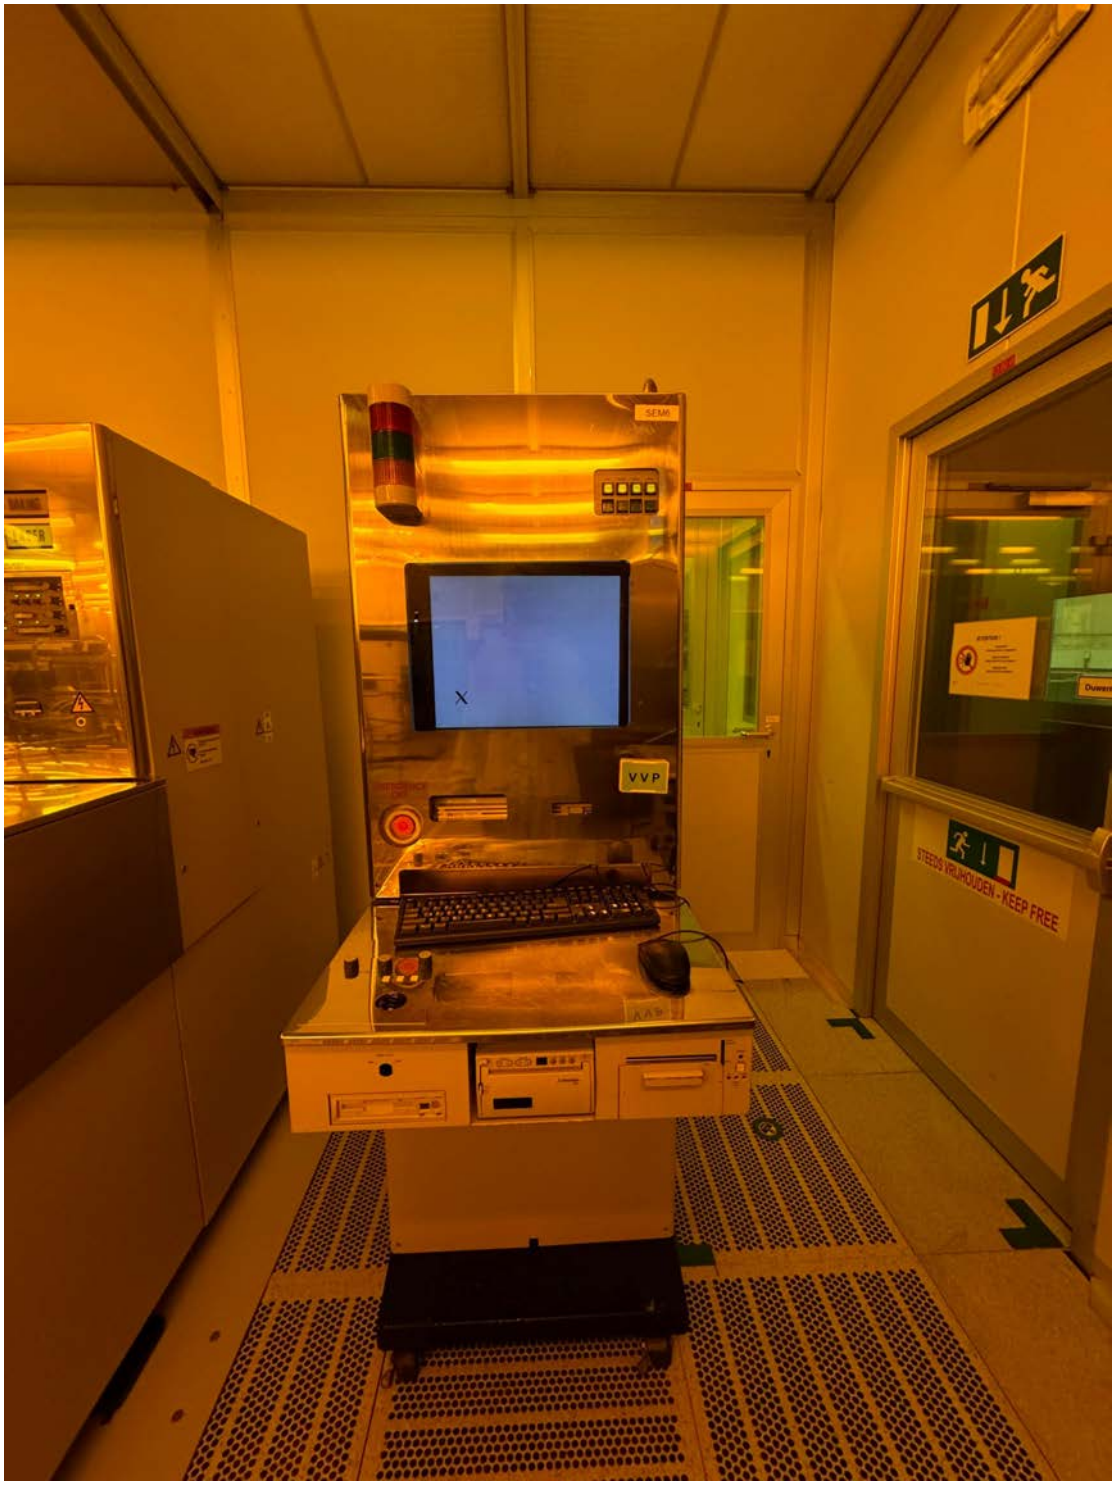
VVP
STEEDS VRIJHOUDEN - KEEP FREE

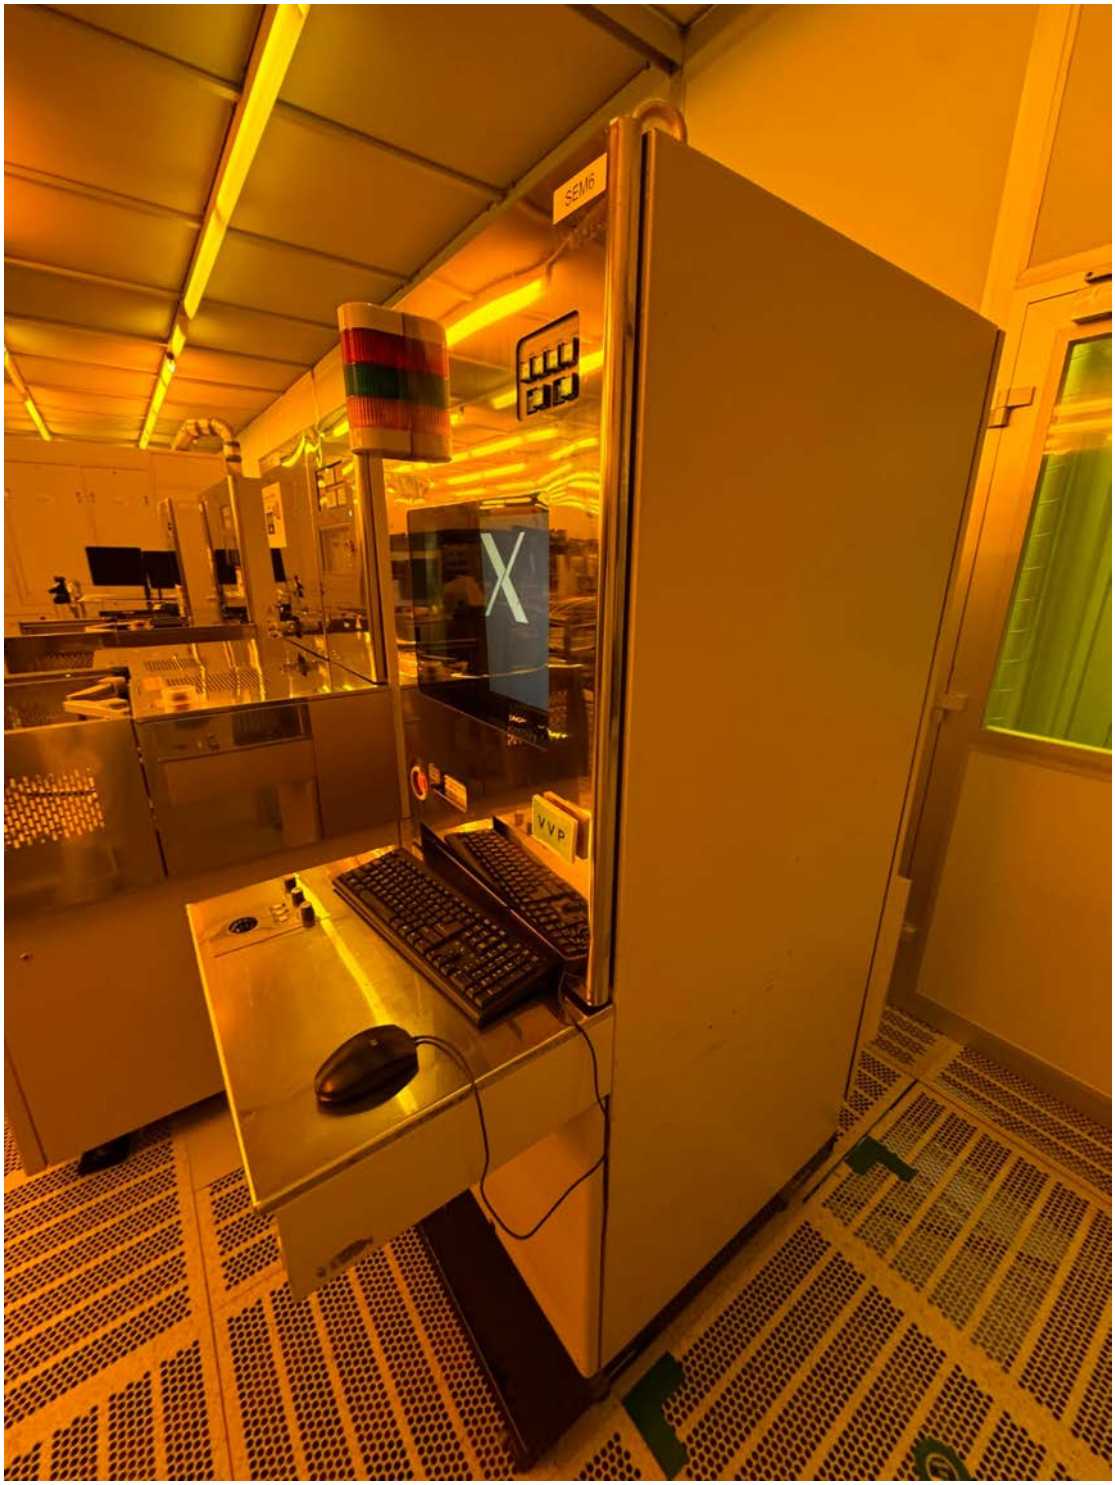
SEM6
VVP

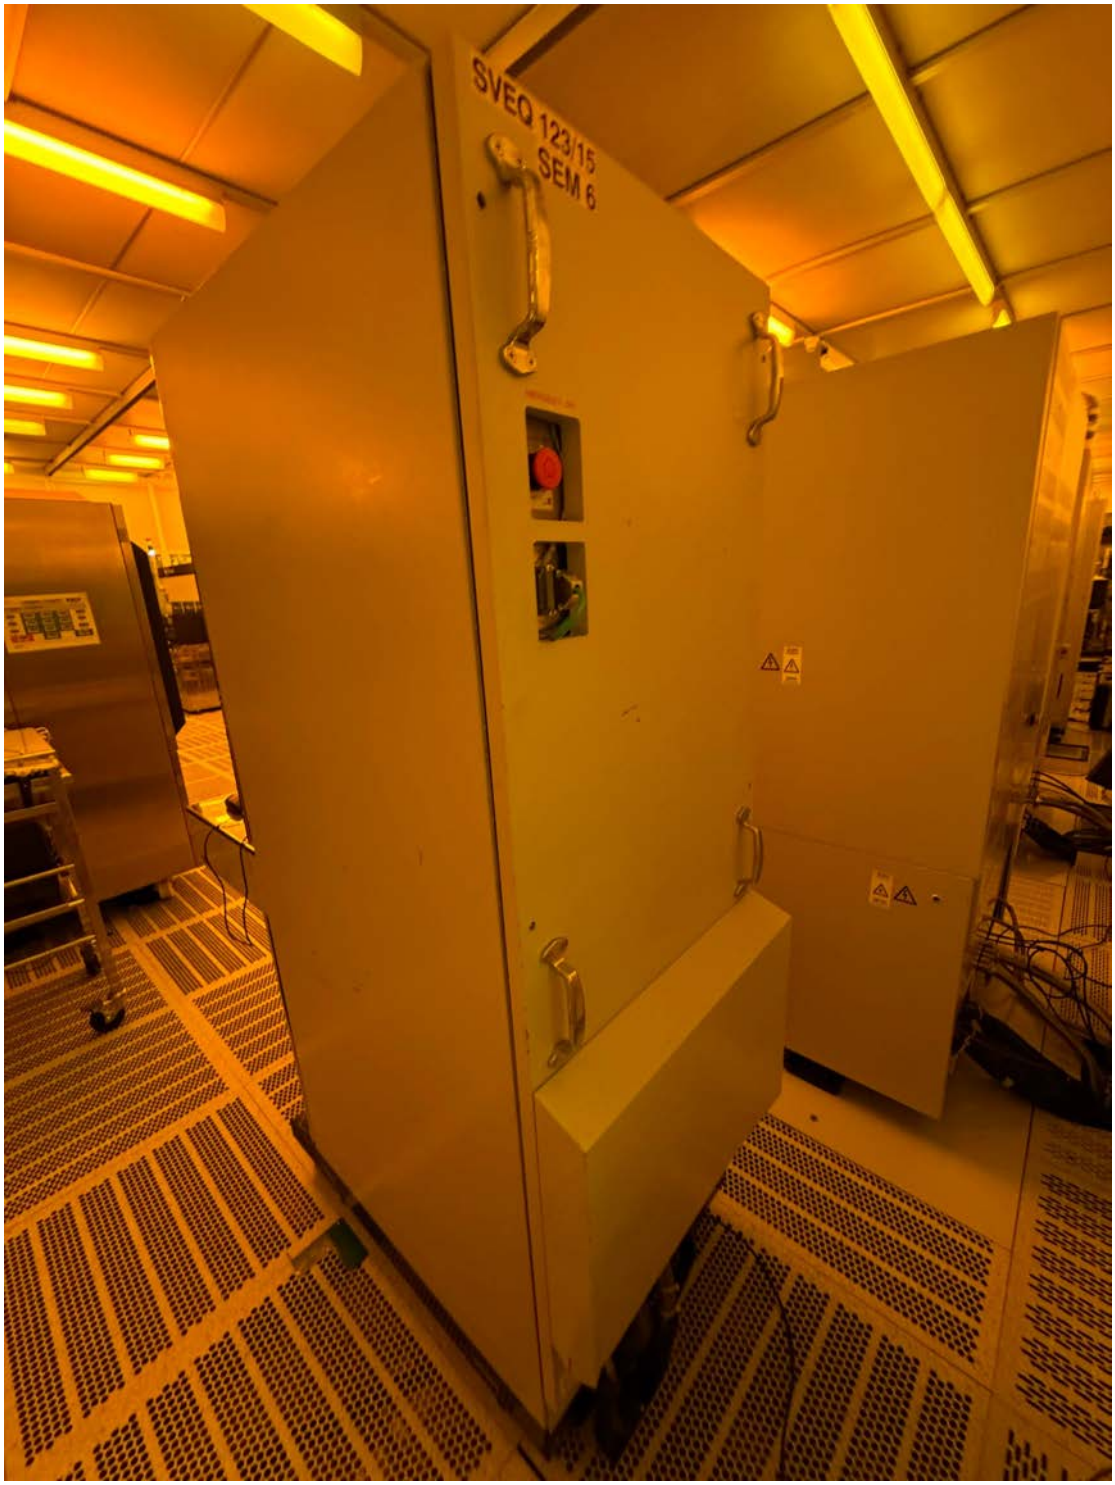
SVEQ 123/15
SEM 6

SCANNING ELECTRON MICROSCOPE
MODEL S-9220
SERIAL NUMBER 9744-06
DATE 01-02
POWER SUPPLY 208V 60Hz
6kVA SINGLE PHASE
Hitachi, Ltd.
MADE IN JAPAN

S-9220
8 - inch
6 - inch
Tool
POST
LASER

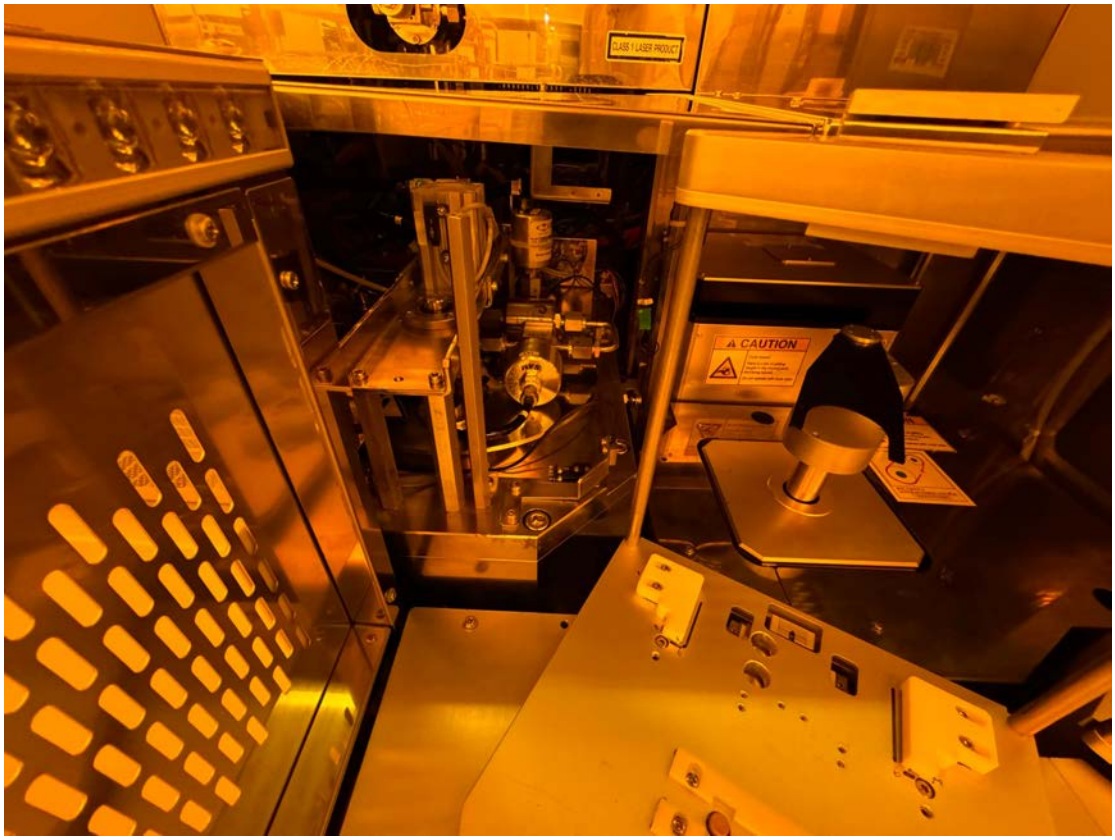
CLASS 1 LASER PRODUCT
CAUTION

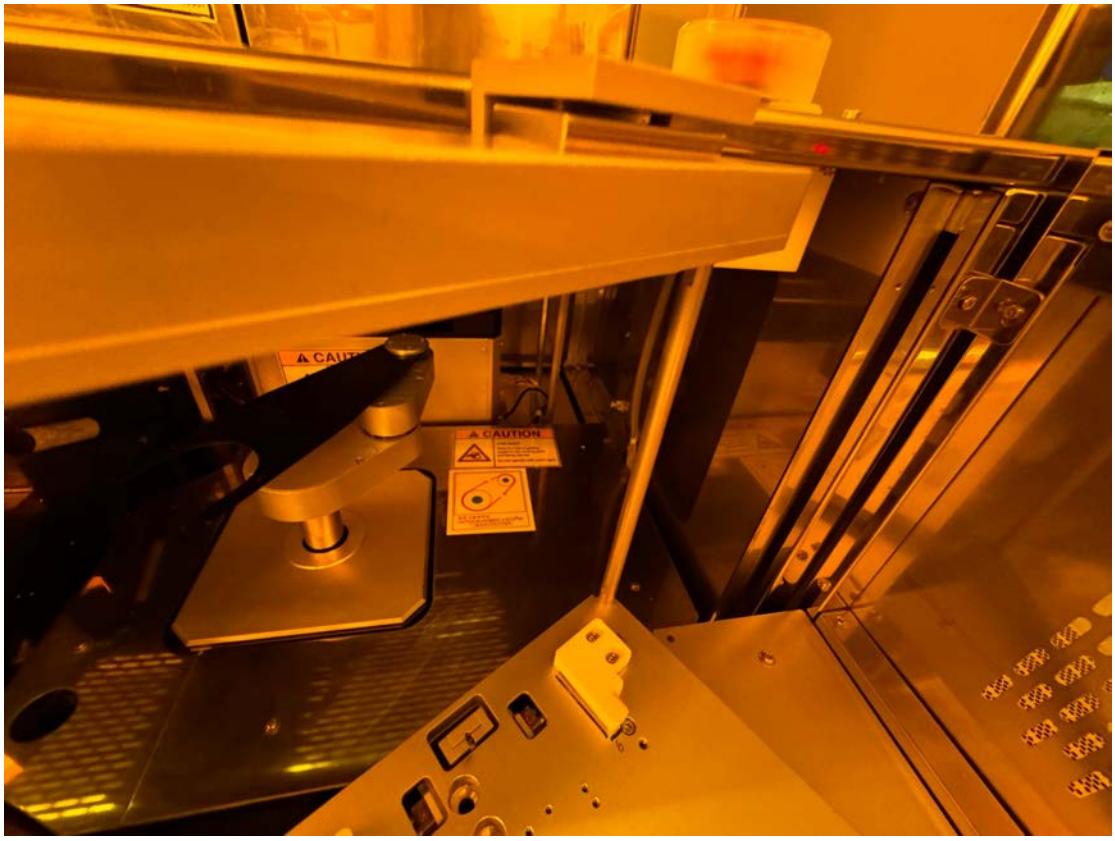
CAUTION

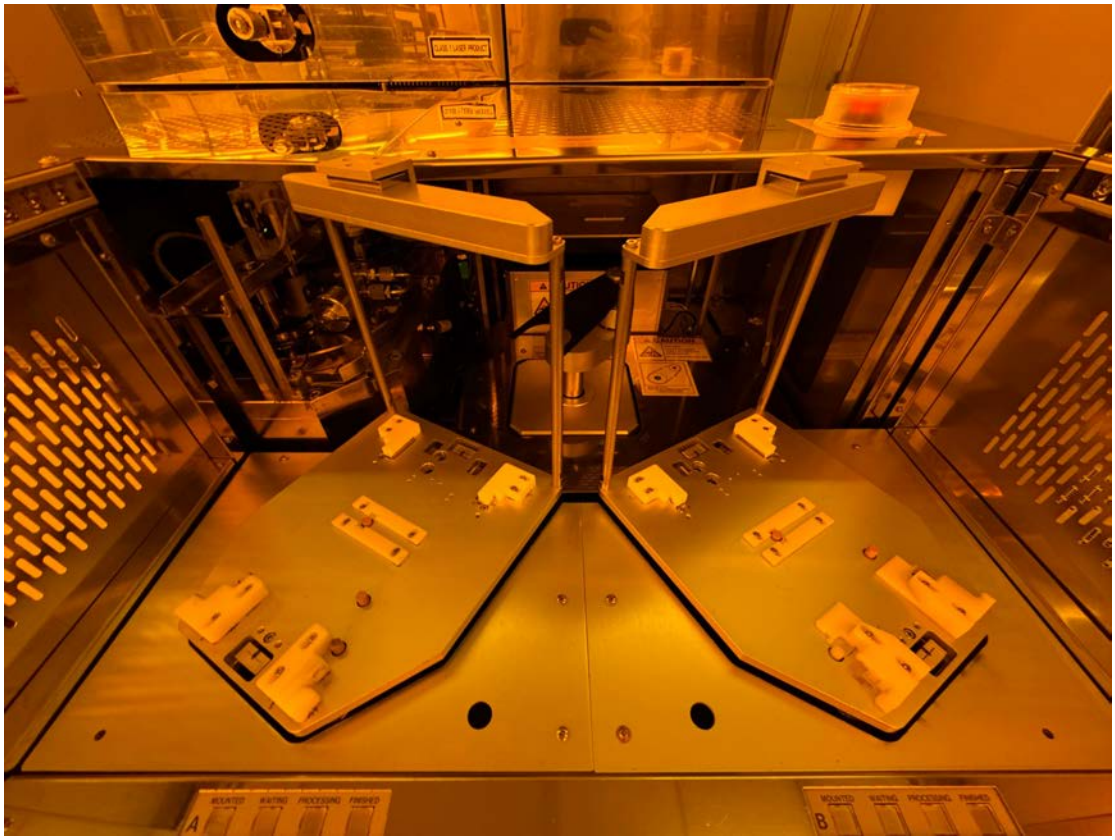

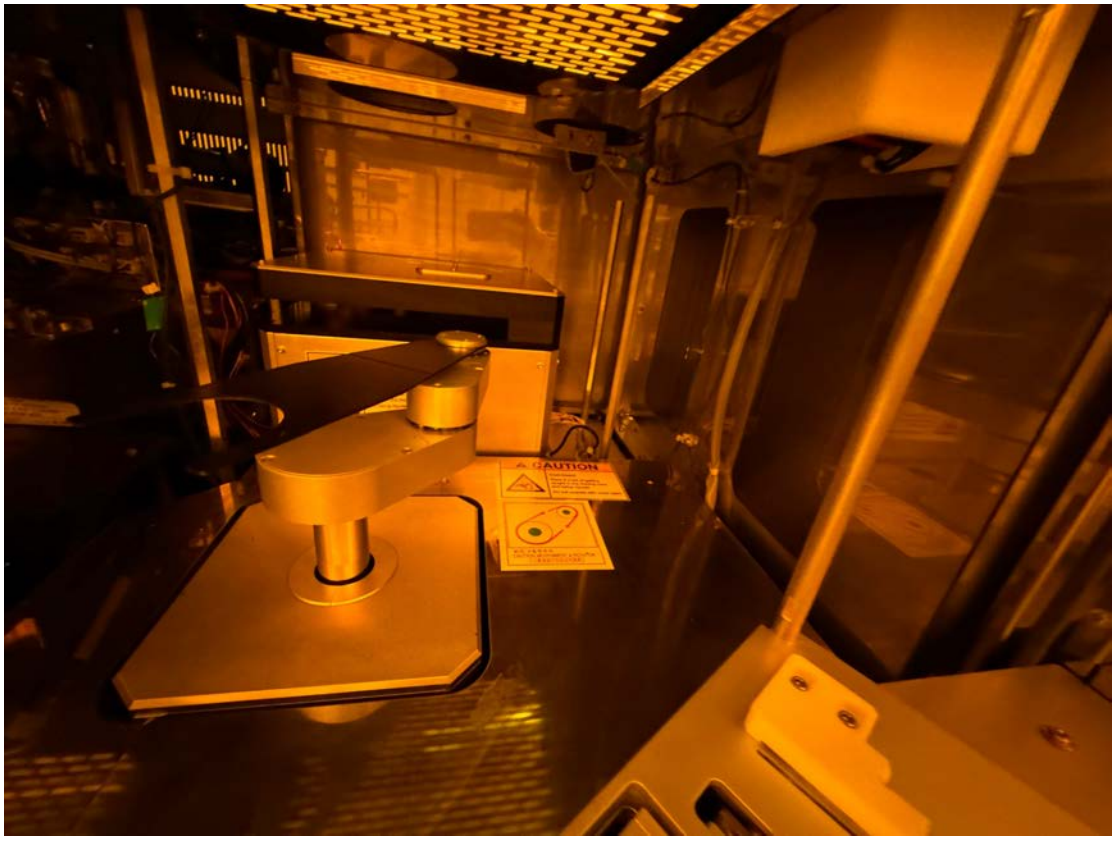

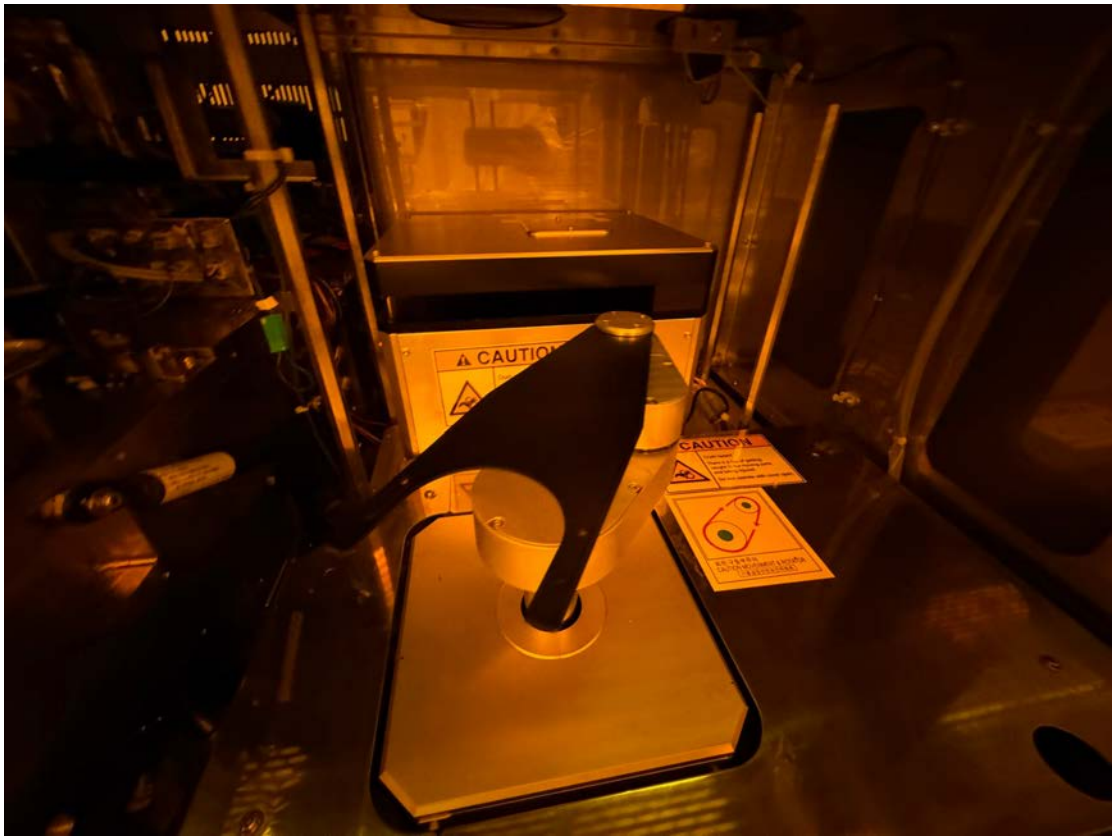
CAUTION
CAUTION

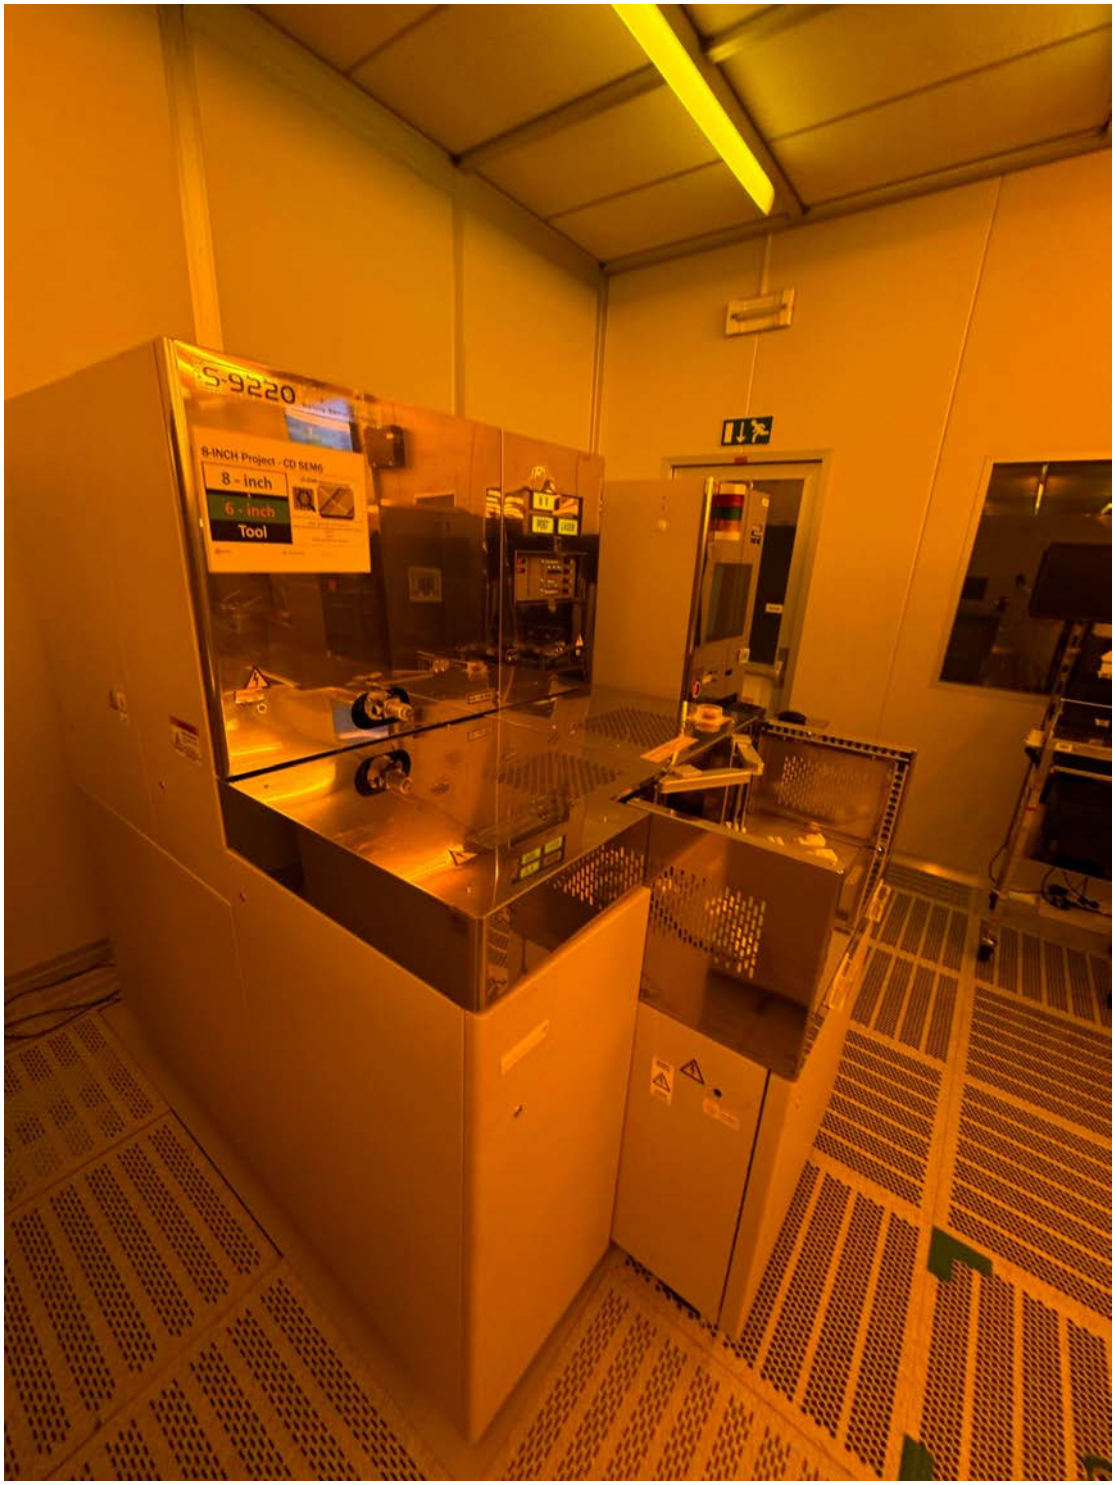
S-9220
8-INCH Project - CD SEM6
8 - inch
6 - inch
Tool

SCANNING ELECTRON MICROSCOPE
MODEL S-9220
SERIAL NUMBER 9727-10
DATE 00-06
POWER SUPPLY 208V 60Hz
6kVA
SINGLE PHASE
Hitachi, Ltd.
MADE IN JAPAN